


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080919\
Data File : VU033687.D
Acq On : 09 Aug 2019 16:07
Operator : JC/SP
Sample : BFB51
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
Title : VOC Analysis
Last Update : Tue Aug 13 04:58:20 2019

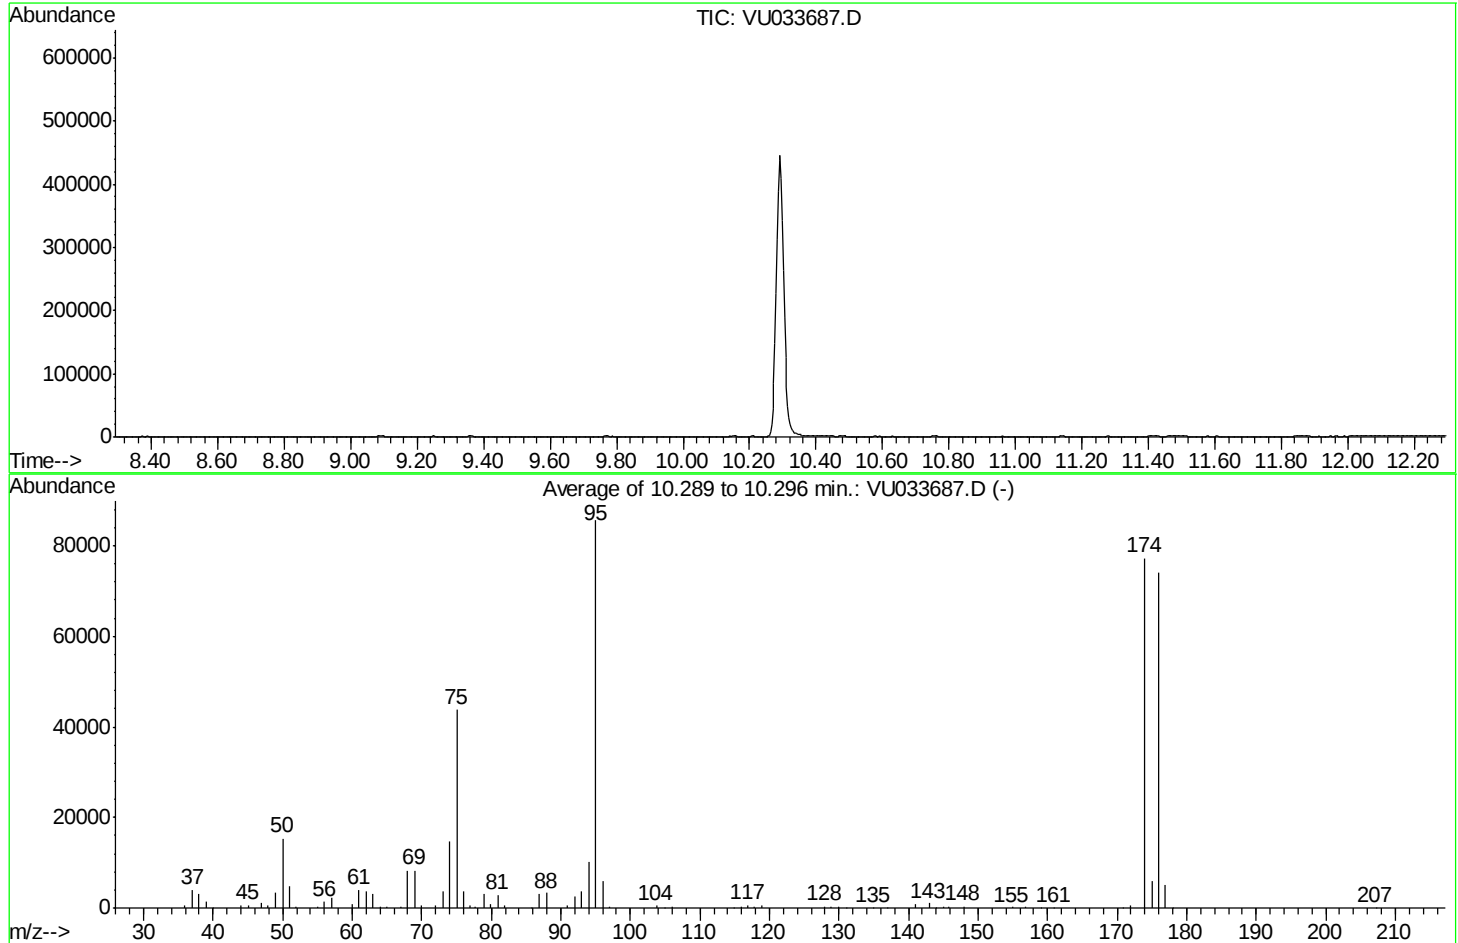

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	15276	PASS
75	95	30	80	51.0	43688	PASS
95	95	100	100	100.0	85616	PASS
96	95	5	9	6.8	5832	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.2	77242	PASS
175	174	5	9	7.6	5871	PASS
176	174	95	101	95.9	74112	PASS
177	176	5	9	6.8	5045	PASS

m/z	Abundance
40.00	200.0
43.90	464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	686.0
37.00	4053.0
38.00	3411.0
39.00	1548.0
39.90	233.0
44.00	1061.0
45.00	714.0
47.00	999.0
47.90	559.0
49.00	3378.0
50.00	15939.0
51.00	5076.0
52.00	222.0
55.00	255.0
56.00	1406.0
57.00	2306.0
60.00	789.0
61.00	4313.0
62.00	3960.0
63.00	3394.0
64.10	433.0
65.00	362.0
67.00	231.0
68.00	8522.0
69.00	8556.0
70.00	693.0
72.00	531.0
73.00	3782.0
74.00	15394.0
75.00	45584.0
76.00	3730.0
76.90	496.0
77.70	283.0
78.90	3016.0
79.90	869.0
80.90	3052.0
82.00	600.0
85.80	118.0
87.00	3288.0
88.00	3420.0
90.90	433.0
92.00	2696.0
93.00	3772.0
94.00	10439.0
95.00	87160.0
96.10	6160.0
97.00	232.0
103.80	488.0
105.00	144.0
106.00	354.0
114.80	103.0
115.90	318.0
116.90	632.0
117.90	368.0
119.00	514.0
128.00	370.0
128.90	209.0
129.90	219.0
131.00	132.0
135.00	168.0
137.00	145.0
141.00	928.0
142.90	1039.0
145.00	116.0
145.80	155.0
148.00	276.0
155.00	246.0
156.90	204.0
158.90	123.0
161.00	100.0
170.90	134.0
172.00	659.0
174.00	77056.0
175.00	6066.0
176.00	73168.0
176.90	5109.0
177.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	694.0
37.00	4178.0
38.00	3337.0
39.00	1662.0
39.90	262.0
44.00	915.0
45.10	693.0
47.00	1149.0
47.90	507.0
49.00	3525.0
50.00	15770.0
51.00	4891.0
51.90	233.0
55.00	289.0
56.00	1363.0
57.00	2392.0
60.00	928.0
61.00	4250.0
62.00	3900.0
63.00	3369.0
64.10	396.0
65.00	401.0
67.00	252.0
68.00	8535.0
69.00	8557.0
70.00	643.0
72.00	483.0
73.00	3707.0
74.00	15237.0
75.00	45096.0
76.00	3625.0
76.90	451.0
77.80	313.0
78.90	3136.0
79.90	836.0
80.90	2949.0
81.90	640.0
86.90	3343.0
88.00	3416.0
90.90	486.0
92.00	2690.0
93.00	3827.0
94.00	10440.0
95.00	88480.0
96.00	6103.0
97.00	185.0
103.80	494.0
104.90	123.0
106.00	339.0
115.90	351.0
116.90	667.0
117.90	341.0
118.90	535.0
128.00	363.0
128.90	216.0
129.90	257.0
131.00	116.0
135.00	155.0
136.90	143.0
141.00	992.0
143.00	1081.0
144.90	159.0
145.80	176.0
147.90	316.0
154.90	247.0
156.90	206.0
158.90	139.0
161.00	156.0
170.90	140.0
172.00	662.0
174.00	79896.0
175.00	6064.0
176.00	76728.0
176.90	5251.0
177.90	149.0
207.20	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	679.0
37.00	3901.0
38.00	3003.0
39.00	1478.0
39.90	274.0
44.00	746.0
45.10	670.0
47.00	1101.0
47.90	458.0
49.00	3393.0
50.00	14121.0
51.00	4311.0
52.00	215.0
54.90	244.0
56.00	1295.0
57.00	2205.0
60.00	917.0
61.00	3720.0
62.00	3516.0
63.00	2961.0
64.00	353.0
65.00	382.0
67.00	238.0
68.00	7768.0
69.00	7890.0
70.00	521.0
72.00	404.0
73.00	3340.0
74.00	13596.0
75.00	40384.0
76.00	3338.0
76.90	395.0
77.80	332.0
78.90	2845.0
79.90	731.0
80.90	2664.0
81.90	608.0
87.00	3056.0
87.90	2985.0
90.90	449.0
92.00	2387.0
93.00	3626.0
94.00	9581.0
95.00	81208.0
96.00	5233.0
96.90	159.0
103.80	410.0
105.90	330.0
115.90	330.0
116.90	593.0
117.80	304.0
118.90	480.0
127.90	291.0
128.90	176.0
129.90	277.0
135.00	125.0
136.90	151.0
141.00	911.0
143.00	1064.0
144.00	100.0
144.90	200.0
145.80	168.0
147.90	283.0
154.90	245.0
156.90	155.0
159.00	135.0
160.90	163.0
170.90	112.0
171.90	590.0
174.00	74776.0
175.00	5484.0
176.00	72440.0
176.90	4777.0
177.90	136.0
207.20	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51