


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080921\
 Data File : VU044399.D
 Acq On : 09 Aug 2021 10:53
 Operator : SY/MD
 Sample : BFB004
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB004

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 10 02:08:42 2021

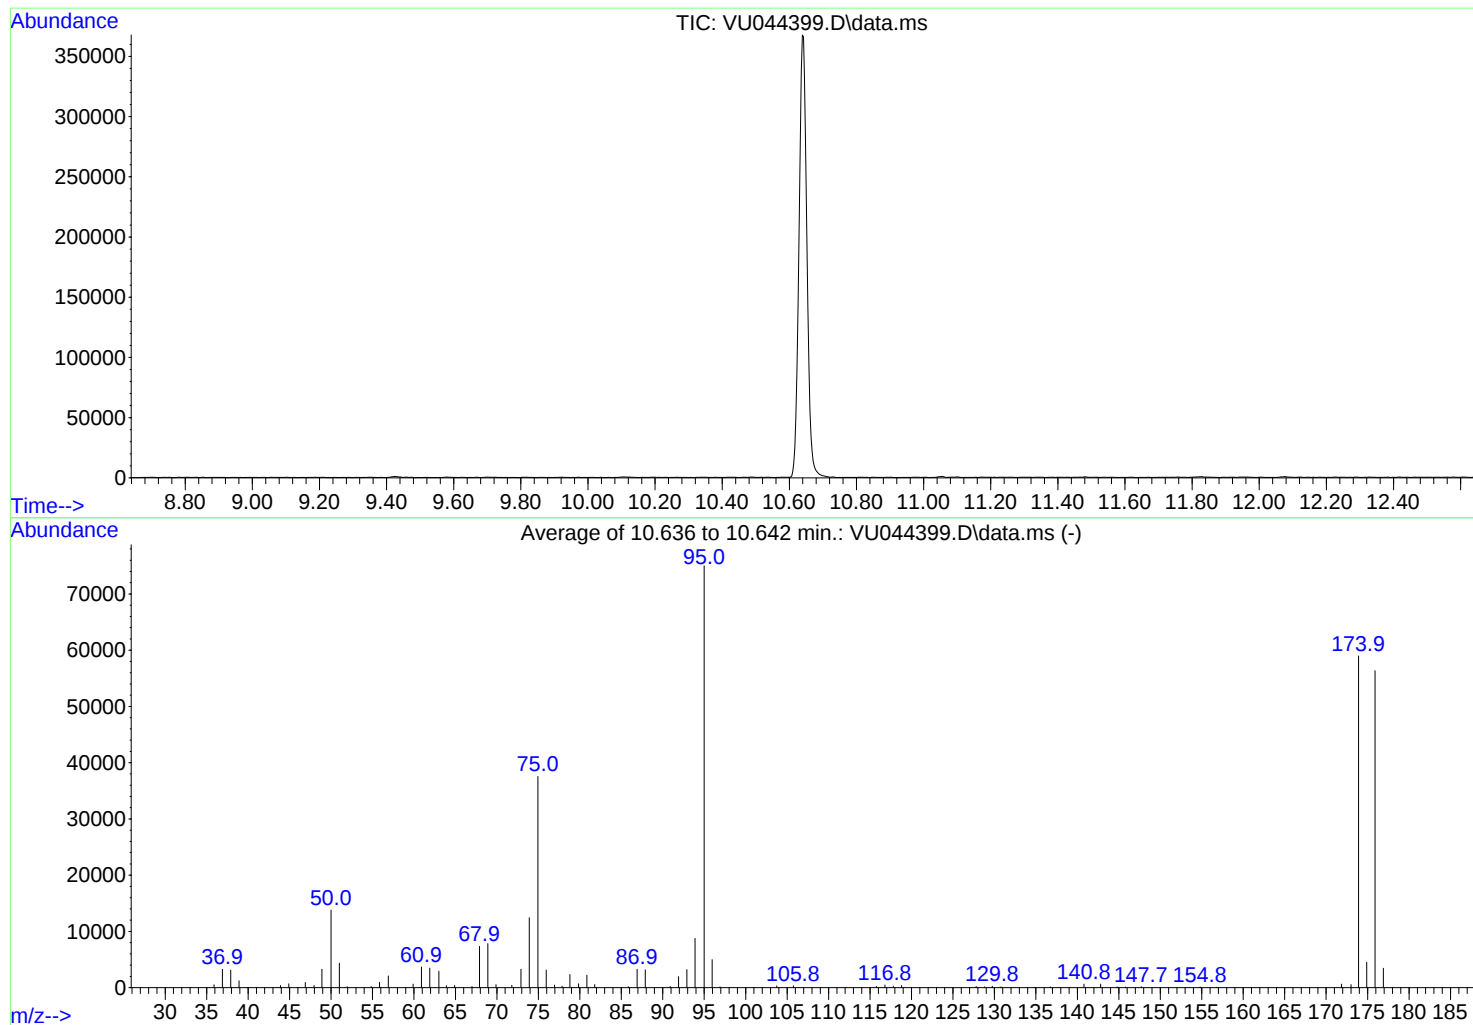

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	13790	PASS
75	95	30	80	50.1	37563	PASS
95	95	100	100	100.0	75000	PASS
96	95	5	9	6.6	4982	PASS
173	174	0.00	2	0.9	534	PASS
174	95	50	120	78.6	58987	PASS
175	174	5	9	7.7	4519	PASS
176	174	95	101	95.5	56352	PASS
177	176	5	9	6.1	3449	PASS

m/z	Abundance
39.90	135.0
43.90	421.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.90	497.0
36.90	3205.0
37.90	3040.0
38.90	1243.0
39.90	136.0
43.90	761.0
44.90	661.0
46.90	890.0
47.90	414.0
48.90	3181.0
50.00	13203.0
51.00	4157.0
52.00	146.0
54.90	194.0
55.90	978.0
56.90	2030.0
59.90	632.0
60.90	3555.0
61.90	3308.0
63.00	2662.0
63.90	343.0
64.90	370.0
67.00	207.0
67.90	6886.0
68.90	7491.0
69.90	548.0
71.80	421.0
72.90	3134.0
73.90	11650.0
74.90	35848.0
75.90	3102.0
77.00	447.0
77.80	294.0
78.80	2244.0
79.80	670.0
80.80	2130.0
81.80	583.0
85.90	139.0
86.90	3066.0
87.90	3113.0
90.90	207.0
91.90	1850.0
92.90	3108.0
93.90	8229.0
95.00	71328.0
95.90	4720.0
96.90	152.0
103.80	319.0
105.70	308.0
115.80	207.0
116.80	485.0
117.80	232.0
118.80	360.0
127.80	181.0
128.80	120.0
129.80	248.0
130.80	132.0
136.70	155.0
140.80	565.0
142.80	597.0
144.80	131.0
145.80	106.0
147.70	177.0
154.80	127.0
171.90	575.0
173.00	460.0
173.90	54752.0
174.90	4156.0
175.90	52048.0
176.90	3242.0
177.80	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.90	515.0
36.90	3253.0
37.90	3113.0
38.90	1186.0
39.80	139.0
43.90	792.0
44.90	672.0
46.90	927.0
48.00	408.0
48.90	3300.0
50.00	13878.0
51.00	4399.0
51.90	196.0
54.80	205.0
55.80	870.0
56.90	2042.0
59.90	604.0
60.90	3699.0
61.90	3520.0
63.00	3105.0
63.90	311.0
64.90	447.0
67.00	197.0
67.90	7642.0
68.90	7904.0
69.90	559.0
71.80	426.0
72.90	3298.0
73.90	12809.0
75.00	38128.0
76.00	3078.0
76.90	447.0
77.90	242.0
78.80	2336.0
79.90	701.0
80.90	2231.0
81.80	501.0
85.80	183.0
86.90	3417.0
87.90	3112.0
90.90	216.0
91.90	2034.0
92.90	3249.0
93.90	9030.0
95.00	76440.0
96.00	5122.0
96.90	130.0
103.70	299.0
105.80	325.0
115.70	228.0
116.80	479.0
117.80	262.0
118.80	359.0
127.80	253.0
128.80	153.0
129.70	251.0
130.80	129.0
134.80	114.0
136.80	151.0
140.80	689.0
142.80	618.0
144.80	164.0
145.80	131.0
147.70	181.0
154.80	128.0
156.80	106.0
158.90	101.0
171.80	666.0
173.00	584.0
173.90	61536.0
174.90	4733.0
175.90	58848.0
176.90	3615.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.90	531.0
36.90	3396.0
37.90	3238.0
38.90	1254.0
39.80	138.0
43.90	809.0
44.90	715.0
46.90	938.0
47.90	412.0
48.90	3370.0
50.00	14289.0
51.00	4476.0
51.90	168.0
54.90	212.0
55.90	956.0
56.90	2124.0
59.90	639.0
60.90	3777.0
61.90	3574.0
63.00	3072.0
63.90	357.0
64.90	427.0
67.00	208.0
67.90	7528.0
68.90	8110.0
69.90	559.0
71.80	433.0
72.90	3350.0
73.90	12849.0
74.90	38712.0
75.90	3211.0
77.00	464.0
77.80	285.0
78.80	2421.0
79.80	711.0
80.80	2262.0
81.80	563.0
85.90	173.0
86.90	3347.0
87.90	3282.0
90.90	220.0
91.90	2024.0
92.90	3308.0
93.90	9031.0
95.00	77232.0
95.90	5105.0
96.90	149.0
103.80	314.0
105.80	332.0
115.70	221.0
116.80	521.0
117.80	260.0
118.80	371.0
127.80	231.0
128.80	152.0
129.80	256.0
130.80	154.0
134.80	112.0
136.80	166.0
140.80	650.0
142.80	639.0
144.80	175.0
145.80	141.0
147.70	198.0
154.80	125.0
156.80	103.0
171.90	655.0
173.00	558.0
173.90	60672.0
174.90	4667.0
175.90	58160.0
176.90	3491.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004