

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
 Data File : VU060368.D
 Acq On : 09 Aug 2024 11:37
 Operator : MD/SY
 Sample : VU0809WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 10 04:52:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 10 04:43:24 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	106493	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	112050	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	46214	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	37474	4.483	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.600%
7) Chloroethane-d5	1.911	69	35639	4.728	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.600%
11) 1,1-Dichloroethene-d2	2.560	65	16253	4.569	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.400%
20) 2-Butanone-d5	4.644	46	85856	48.396	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.800%
24) Chloroform-d	5.055	84	78252	4.728	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.695	65	38241	4.982	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
32) Benzene-d6	5.721	84	150247	4.446	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.685	67	49873	4.758	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.894	98	120829	4.005	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	8.177	79	14923	4.404	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.000%
46) 2-Hexanone-d5	8.631	63	67035	44.577	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.160%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	40714	4.734	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	43969	5.165	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						Qvalue
35) Methylcyclohexane	6.688	83	11456	1.039	ug/L #	18
37) 1,2-Dichloropropane	6.682	63	4959	0.565	ug/L #	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
Data File : VU060368.D
Acq On : 09 Aug 2024 11:37
Operator : MD/SY
Sample : VU0809WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 10 04:52:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 10 04:43:24 2024
Response via : Initial Calibration

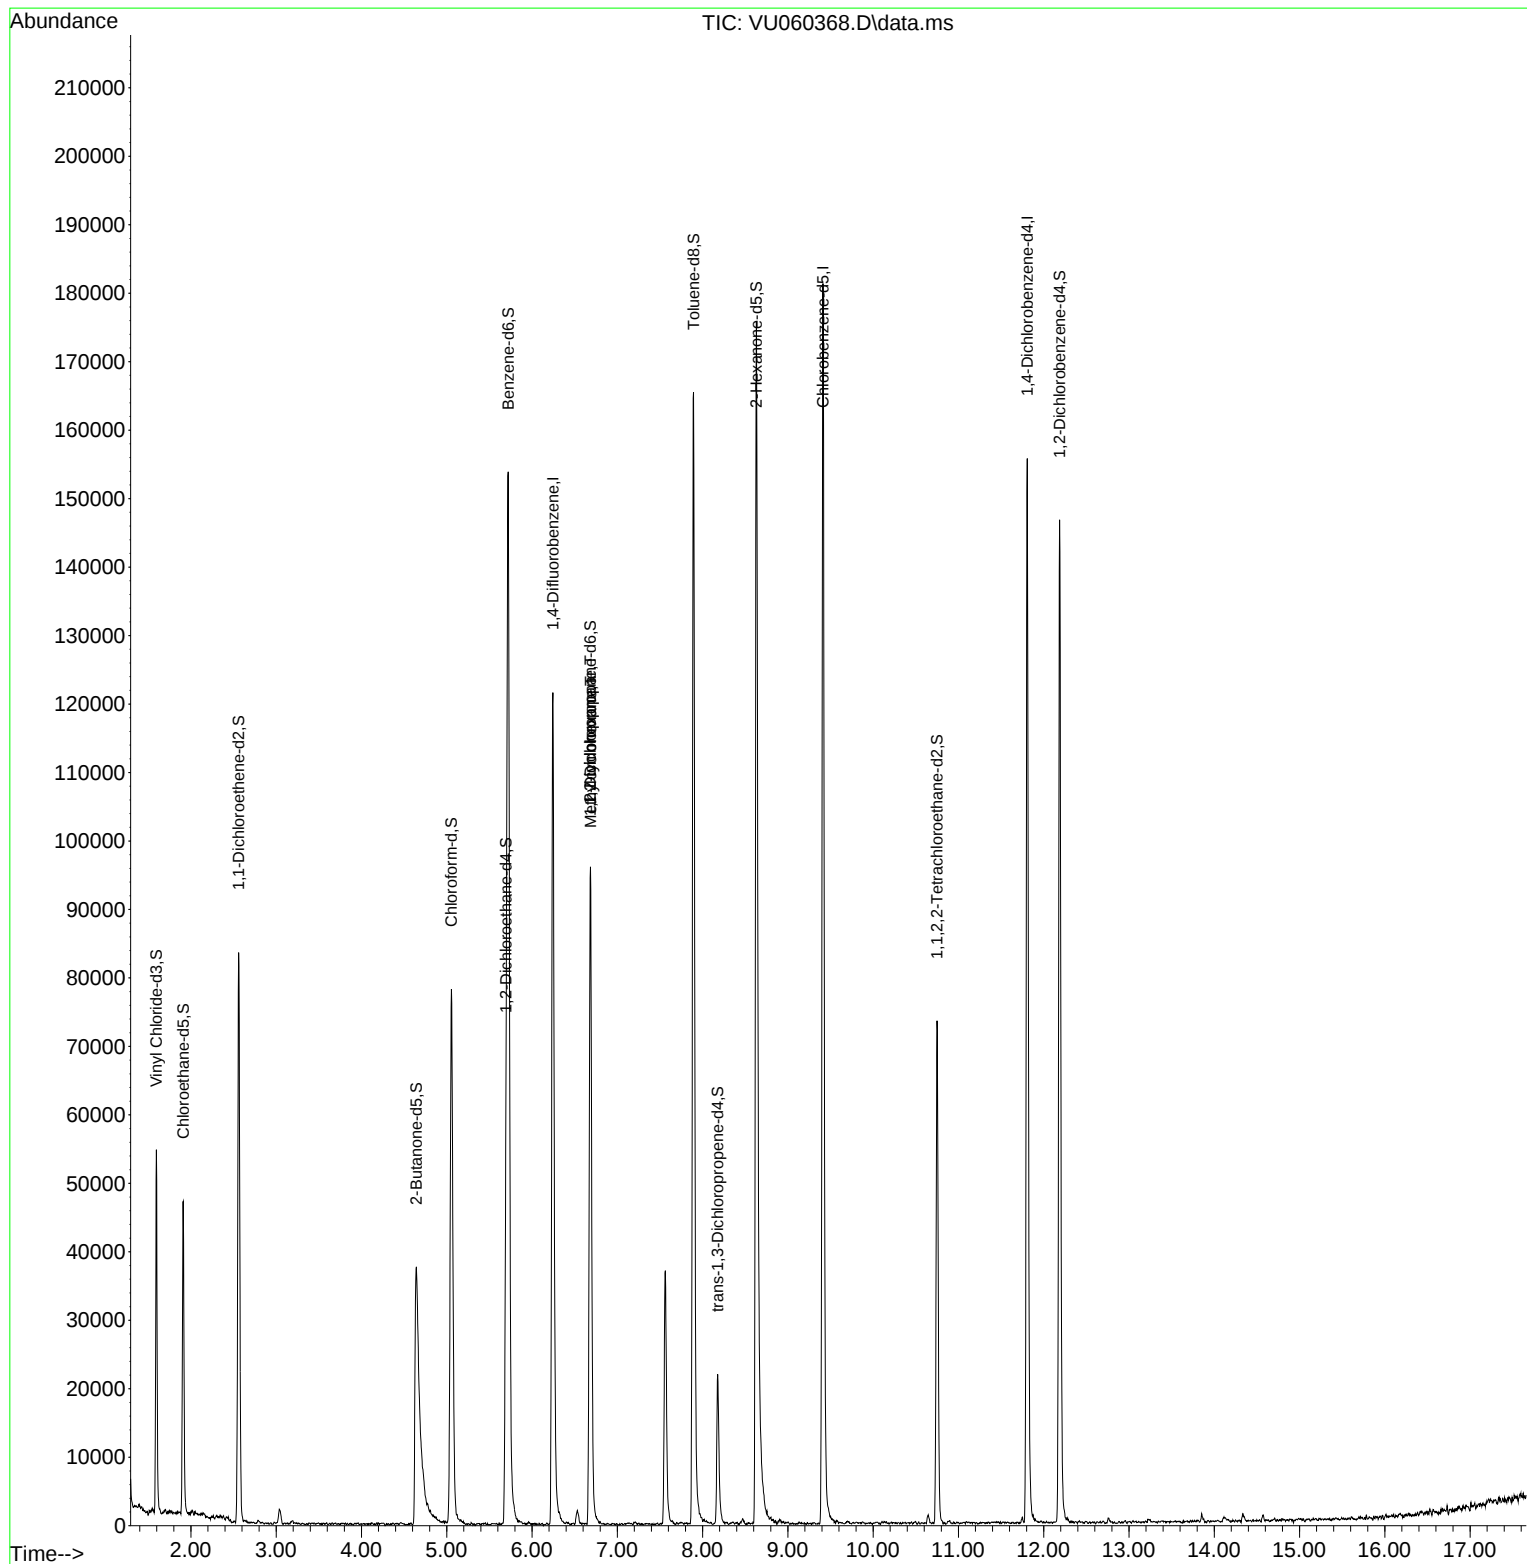

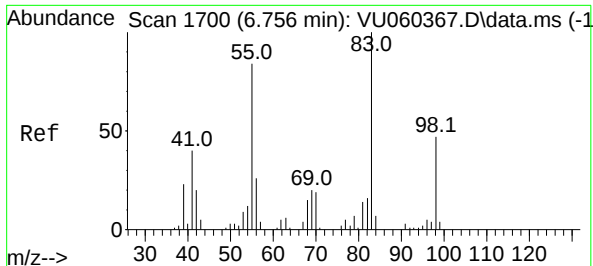

#35

Methylcyclohexane

Concen: 1.039 ug/L





RT: 6.688 min Scan# 1679

Delta R.T. -0.068 min

Lab File: VU060368.D

Acq: 09 Aug 2024 11:37

Tgt Ion:	83	Resp:	11456
Ion	Ratio	Lower	Upper
83	100		
55	0.0	62.4	93.6#
98	1.3	37.3	55.9#

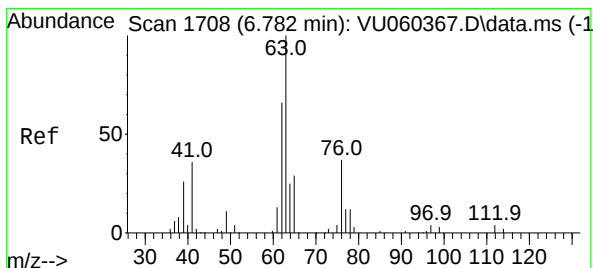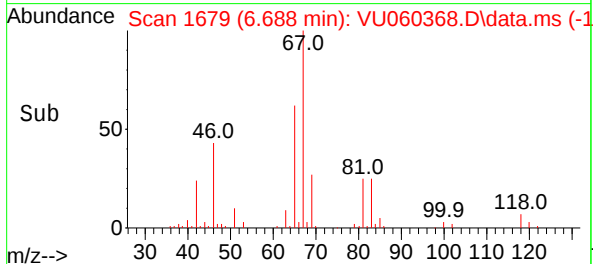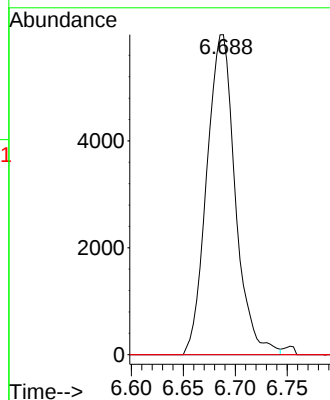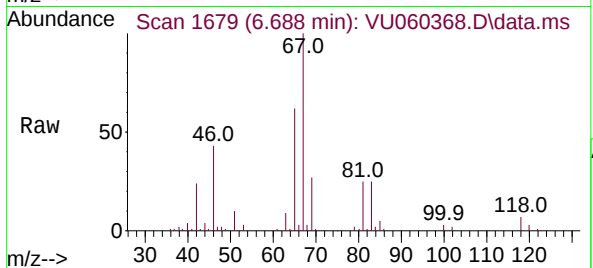

#37

1,2-Dichloropropane

Concen: 0.565 ug/L

RT: 6.682 min Scan# 1677

Delta R.T. -0.100 min

Lab File: VU060368.D

Acq: 09 Aug 2024 11:37

Tgt Ion:	63	Resp:	4959
Ion	Ratio	Lower	Upper
63	100		
112	0.0	3.3	4.9#

