

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
 Data File : VU060382.D
 Acq On : 09 Aug 2024 19:27
 Operator : MD/SY
 Sample : P3401-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF5

Quant Time: Aug 10 04:57:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 10 04:43:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	98232	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	105318	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	45643	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	33735	4.375	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.600%
7) Chloroethane-d5	1.907	69	33554	4.826	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.560	65	14161	4.315	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.400%
20) 2-Butanone-d5	4.634	46	94425	57.703	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.400%
24) Chloroform-d	5.055	84	74713	4.893	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.698	65	36673	5.180	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	5.721	84	139251	4.384	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	6.685	67	48523	4.925	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.894	98	110116	3.883	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.600%
43) trans-1,3-Dichloroprop...	8.177	79	13986	4.391	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.631	63	65303	46.201	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.400%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	40449	5.004	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	44848	5.334	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds					Qvalue	
13) Acetone	2.647	43	54822	49.060	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
Data File : VU060382.D
Acq On : 09 Aug 2024 19:27
Operator : MD/SY
Sample : P3401-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF5

Quant Time: Aug 10 04:57:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 10 04:43:24 2024
Response via : Initial Calibration

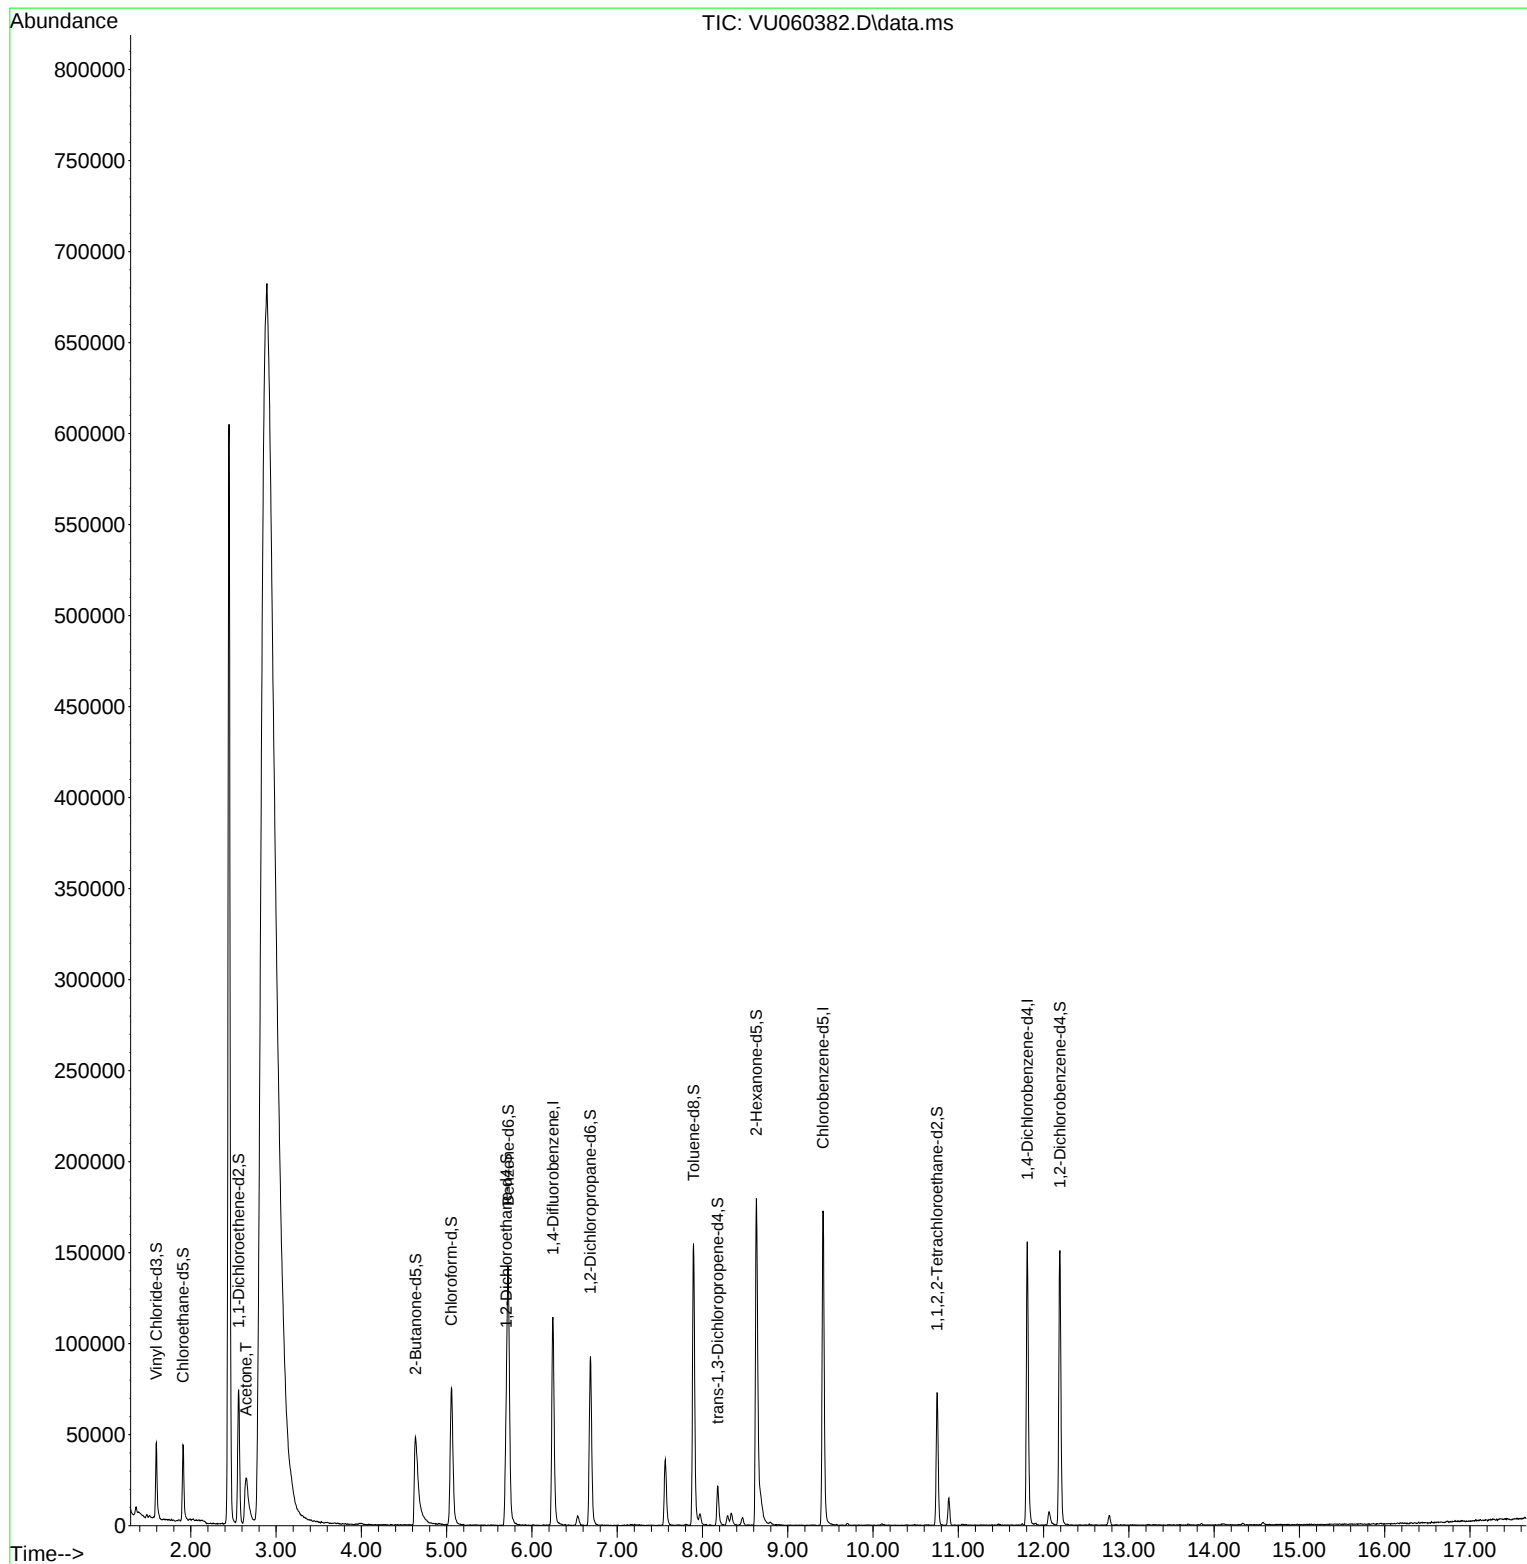

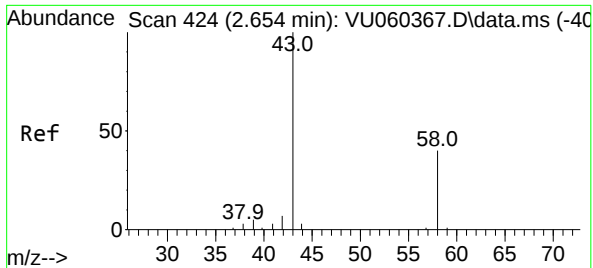

#13
 Acetone
 Concen: 49.060 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. -0.007 min
 Lab File: VU060382.D
 Acq: 09 Aug 2024 19:27

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF5

Tgt Ion: 43 Resp: 54822
 Ion Ratio Lower Upper
 43 100
 58 38.0 0.0 78.8

