

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
 Data File : VU060385.D
 Acq On : 09 Aug 2024 20:36
 Operator : MD/SY
 Sample : P3401-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GG4

Quant Time: Aug 10 04:58:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 10 04:43:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	102741	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	108241	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	45908	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	33787	4.190	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%
7) Chloroethane-d5	1.911	69	32838	4.516	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.400%
11) 1,1-Dichloroethene-d2	2.563	65	14420	4.201	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.000%
20) 2-Butanone-d5	4.634	46	95478	55.785	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.580%
24) Chloroform-d	5.055	84	75104	4.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	5.695	65	36219	4.891	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	5.721	84	143382	4.392	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	6.682	67	49283	4.867	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.894	98	112208	3.850	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.000%
43) trans-1,3-Dichloroprop...	8.174	79	13927	4.255	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.631	63	69807	48.054	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.100%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	39863	4.798	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	45499	5.380	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds					Qvalue	
13) Acetone	2.653	43	19170	16.402	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
Data File : VU060385.D
Acq On : 09 Aug 2024 20:36
Operator : MD/SY
Sample : P3401-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GG4

Quant Time: Aug 10 04:58:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 10 04:43:24 2024
Response via : Initial Calibration

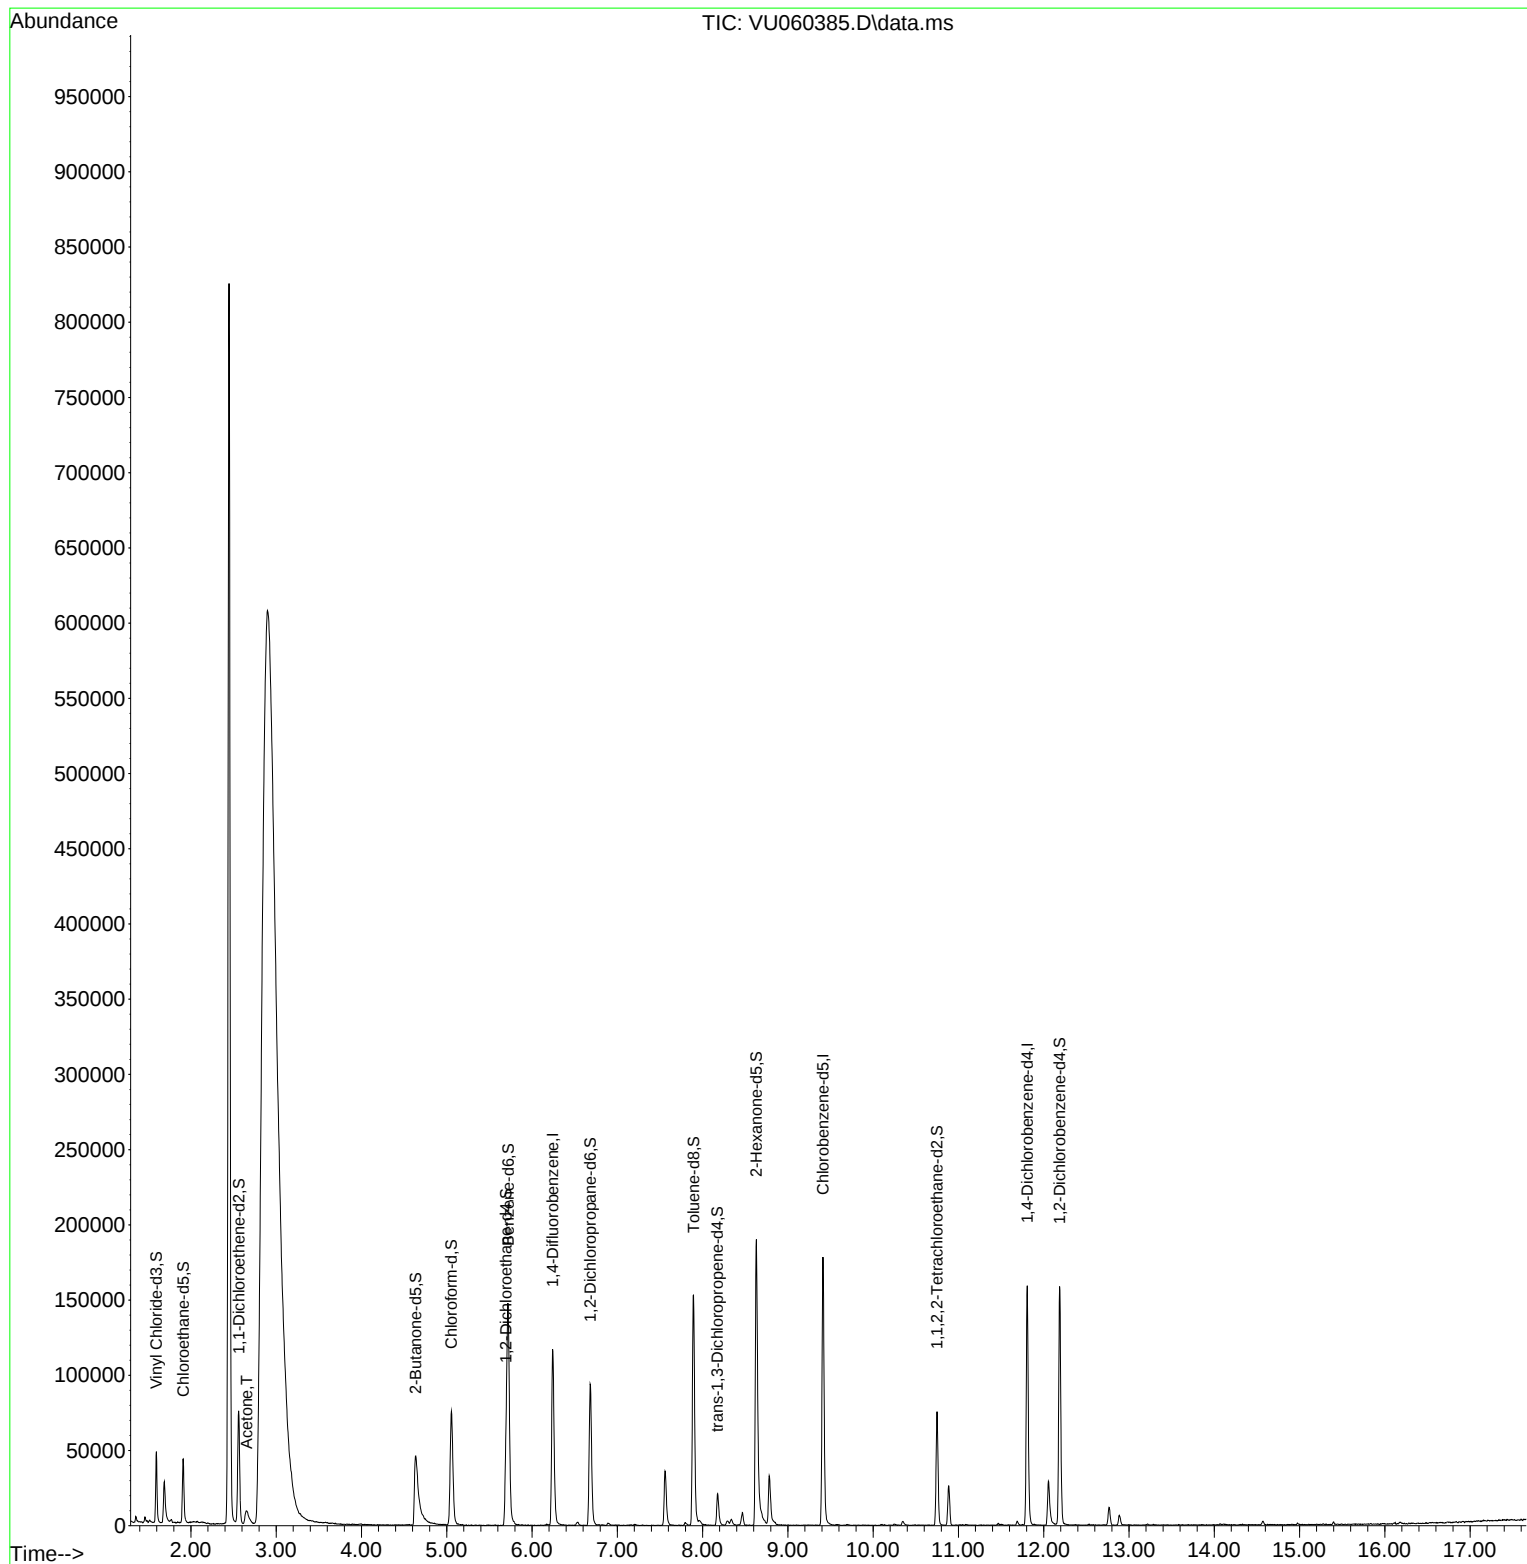

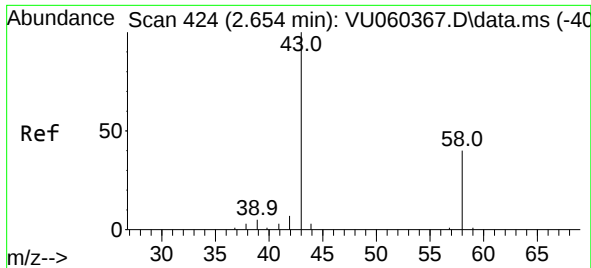

#13

Acetone

Concen: 16.402 ug/L

RT: 2.653 min Scan# 41

Delta R.T. -0.000 min

Lab File: VU060385.D


Acq: 09 Aug 2024 20:36

Instrument :

MSVOA_U

ClientSampleId :

E1GG4

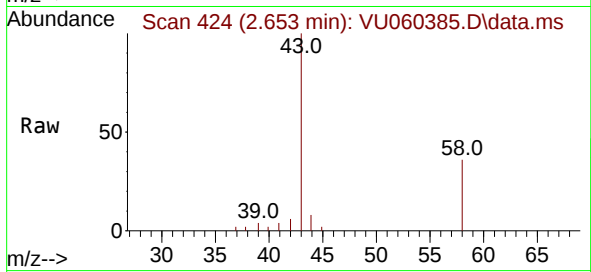

Tgt Ion: 43 Resp: 19170

Ion Ratio Lower Upper

43 100

58 37.8 0.0 78.8

