


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080924\
Data File : VU060366.D
Acq On : 09 Aug 2024 10:18
Operator : MD/SY
Sample : BFB182
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB182

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 10 05:58:50 2024

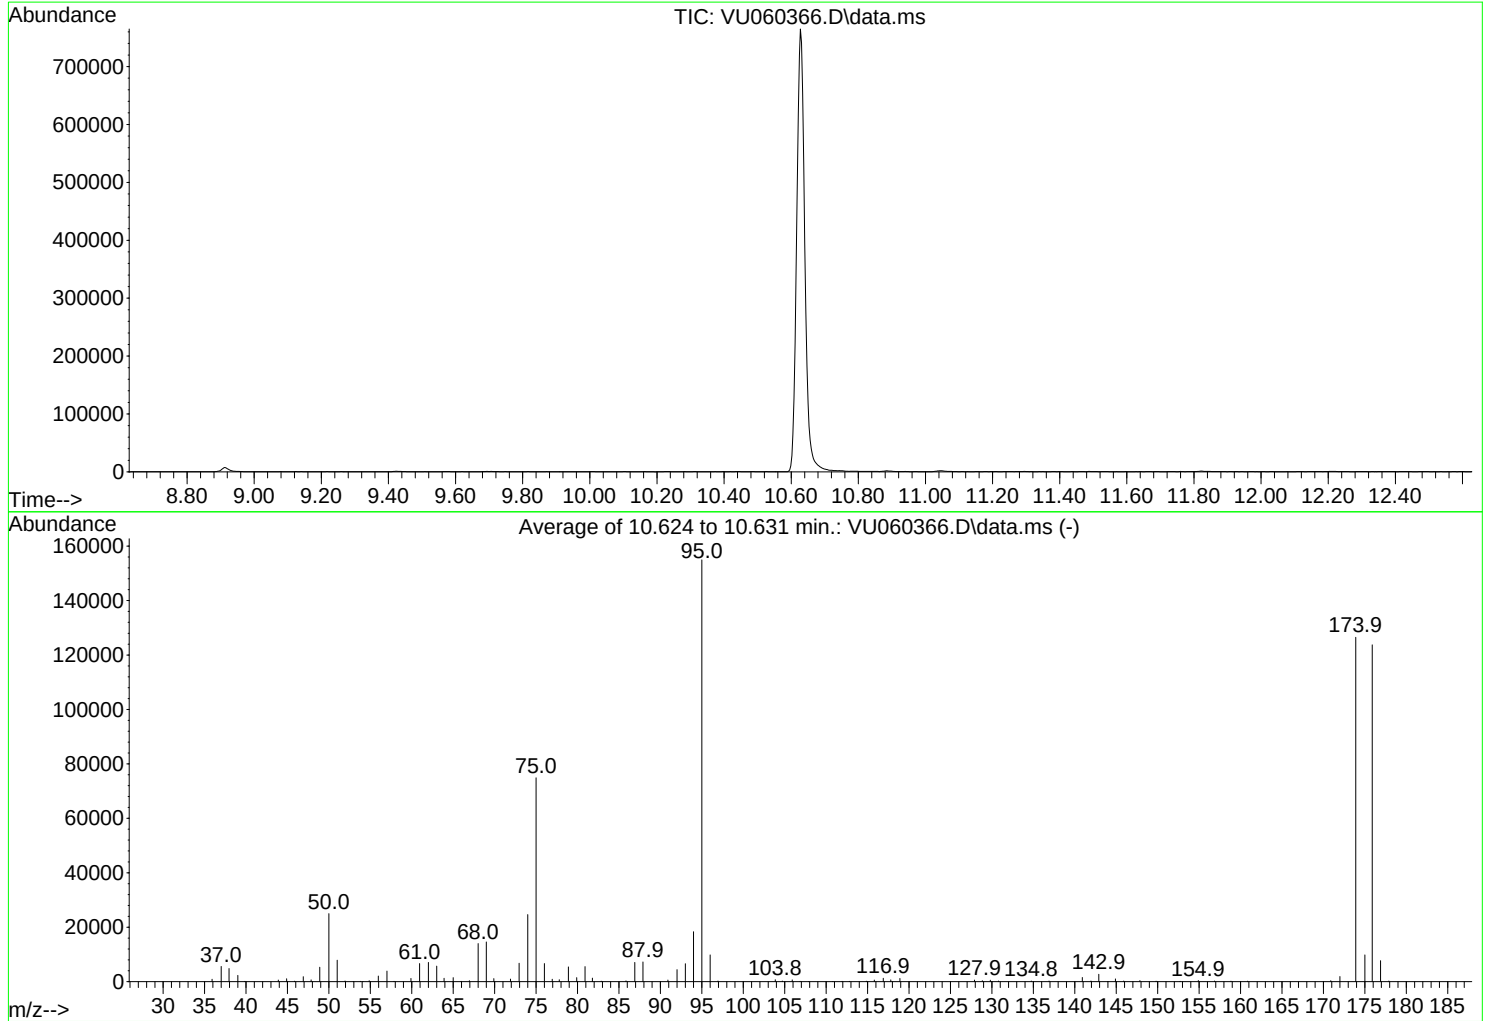

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	24995	PASS
75	95	30	80	48.3	74891	PASS
95	95	100	100	100.0	154965	PASS
96	95	5	9	6.4	9842	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.7	126531	PASS
175	174	5	9	7.8	9820	PASS
176	174	95	101	97.8	123757	PASS
177	176	5	9	6.2	7730	PASS

m/z	Abundance
39.90	115.0
43.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.90	905.0
37.00	5611.0
37.90	4789.0
39.00	2301.0
39.90	247.0
43.90	845.0
44.90	1027.0
45.80	173.0
46.90	1851.0
47.90	665.0
48.90	5206.0
50.00	23936.0
51.00	8139.0
51.90	238.0
53.80	146.0
54.90	324.0
55.90	2037.0
57.00	3869.0
57.90	167.0
59.90	1186.0
60.90	6410.0
62.00	6889.0
63.00	5869.0
63.90	1199.0
65.00	1540.0
65.90	107.0
66.90	364.0
68.00	13840.0
69.00	14207.0
69.90	1182.0
71.90	854.0
72.90	6581.0
74.00	24448.0
75.00	73320.0
76.00	6500.0
77.00	856.0
77.80	672.0
78.90	5293.0
79.90	1443.0
80.90	5605.0
81.80	1245.0
82.80	155.0
85.80	348.0
86.90	6730.0
87.90	6980.0
90.90	598.0
92.00	4429.0
93.00	6347.0
94.00	17992.0
95.00	150272.0
96.00	9855.0
97.00	304.0
103.90	646.0
104.70	256.0
105.90	664.0
107.90	106.0
111.90	113.0
112.80	132.0
114.80	175.0
115.80	584.0
116.90	1218.0
117.80	644.0
118.90	1208.0
127.90	582.0
128.80	326.0
129.80	518.0
130.80	213.0
134.70	230.0
136.90	258.0
140.90	1474.0
141.90	253.0
142.90	2802.0
144.00	149.0
144.90	1097.0
145.90	181.0
147.80	366.0
149.80	125.0
152.70	114.0
155.00	388.0
156.80	269.0
158.90	160.0
160.80	190.0
170.90	340.0
172.00	1870.0
173.90	120832.0
175.00	9435.0
175.90	118168.0
176.90	7463.0
177.90	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.90	884.0
37.00	5760.0
38.00	4932.0
39.00	2425.0
39.90	225.0
44.00	842.0
44.90	1125.0
45.80	220.0
46.90	1855.0
47.80	634.0
48.90	5399.0
50.00	25712.0
51.00	8157.0
51.90	253.0
52.90	111.0
53.80	120.0
54.80	325.0
56.00	2131.0
57.00	4033.0
57.90	129.0
59.90	1185.0
61.00	6807.0
62.00	7358.0
63.00	5795.0
63.90	1315.0
65.00	1567.0
65.90	143.0
66.90	368.0
68.00	14488.0
69.00	15074.0
69.90	1162.0
71.90	1014.0
73.00	6930.0
74.00	25352.0
75.00	77296.0
76.00	6893.0
76.90	934.0
77.80	707.0
78.90	5583.0
79.90	1485.0
80.90	5684.0
81.80	1341.0
82.90	164.0
85.90	275.0
86.90	7260.0
87.90	7512.0
90.90	593.0
92.00	4552.0
93.00	6774.0
94.00	19064.0
95.00	159424.0
96.00	10140.0
97.00	273.0
103.90	738.0
104.70	274.0
105.90	667.0
106.80	141.0
110.80	109.0
111.90	140.0
112.80	162.0
114.80	198.0
115.80	650.0
116.90	1291.0
117.80	663.0
118.90	1218.0
127.90	623.0
128.90	379.0
129.80	575.0
130.80	247.0
134.80	256.0
136.90	272.0
140.90	1604.0
141.90	269.0
142.90	2791.0
144.00	119.0
144.90	1058.0
145.90	244.0
147.90	427.0
149.80	174.0
152.70	127.0
154.90	401.0
156.80	264.0
158.80	150.0
160.80	193.0
170.90	382.0
172.00	1997.0
173.90	130176.0
175.00	10113.0
175.90	127752.0
176.90	7930.0
177.90	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
35.90	883.0
37.00	5351.0
37.90	4679.0
39.00	2248.0
39.80	200.0
43.90	851.0
44.90	1077.0
45.90	220.0
46.90	1743.0
47.80	609.0
48.90	5187.0
50.00	25336.0
51.00	7355.0
52.00	295.0
53.00	133.0
53.80	109.0
54.10	120.0
54.80	361.0
56.00	1976.0
57.00	3764.0
57.80	111.0
59.90	1169.0
61.00	6728.0
62.00	6948.0
63.00	5386.0
63.90	1156.0
65.00	1401.0
66.00	156.0
67.00	319.0
68.00	13643.0
69.00	14502.0
69.90	1105.0
71.90	931.0
73.00	6770.0
74.00	24096.0
75.00	74056.0
76.00	6503.0
76.90	903.0
77.80	681.0
78.90	5434.0
79.90	1427.0
80.90	5357.0
81.80	1288.0
82.90	160.0
85.90	196.0
86.90	7166.0
87.90	7246.0
90.90	533.0
92.00	4220.0
93.00	6593.0
94.00	17984.0
95.00	155200.0
96.00	9530.0
96.90	230.0
103.80	737.0
104.70	232.0
105.90	638.0
106.90	178.0
110.80	114.0
111.90	163.0
112.80	150.0
114.90	238.0
115.80	595.0
116.90	1228.0
117.80	628.0
118.90	1119.0
127.90	583.0
128.80	355.0
129.80	556.0
130.80	241.0
134.80	278.0
136.90	237.0
140.90	1577.0
142.00	250.0
142.90	2448.0
144.90	918.0
145.90	279.0
147.90	405.0
149.80	202.0
152.70	113.0
154.80	364.0
156.90	251.0
158.80	148.0
160.90	188.0
170.90	365.0
172.00	1880.0
173.90	128584.0
175.00	9913.0
175.90	125352.0
176.90	7798.0
177.90	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182