

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081018\
 Data File : VU026050.D
 Acq On : 10 Aug 2018 17:57
 Operator : MD/SY
 Sample : J4361-24DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.619	5	9	14	rBB3	243	250	0.002%	0.003%
2	0.667	21	24	28	rBV2	254	227	0.001%	0.002%
3	0.696	32	33	34	rBV2	135	37	0.000%	0.000%
4	0.754	48	51	53	rBV2	261	163	0.001%	0.002%
5	0.770	54	56	60	rVB	190	94	0.001%	0.001%
6	0.799	61	65	66	rBV	458	303	0.002%	0.003%
7	0.995	123	126	129	rBV3	201	174	0.001%	0.002%
8	1.085	137	154	171	rBV	251013	295777	19.11%	3.049%
9	1.397	244	251	264	rBV	139671	145594	9.41%	1.501%
10	1.670	329	336	350	rVB	95962	122054	7.89%	1.258%
11	2.268	513	522	534	rVB	234786	349704	22.59%	3.604%
12	2.796	683	686	688	rBV	356	179	0.001%	0.002%
13	2.837	691	699	714	rVB	4555	9282	0.60%	0.096%
14	2.966	737	739	741	rBV3	300	124	0.001%	0.001%
15	3.043	761	763	767	rBV	313	245	0.002%	0.003%
16	3.262	828	831	834	rBV	298	252	0.002%	0.003%
17	3.333	850	853	857	rVB2	627	510	0.003%	0.005%
18	3.365	857	863	865	rBV3	391	376	0.002%	0.004%
19	3.381	865	868	869	rBV	340	178	0.001%	0.002%
20	3.423	876	881	883	rBV	287	269	0.002%	0.003%
21	3.622	940	943	947	rBV	233	160	0.001%	0.002%
22	3.645	948	950	954	rVB3	372	187	0.001%	0.002%
23	3.693	964	965	966	rBV3	96	21	0.000%	0.000%
24	3.712	969	971	974	rVV	206	86	0.001%	0.001%
25	3.728	974	976	978	rVV	217	141	0.001%	0.001%
26	3.751	982	983	985	rBV	188	56	0.000%	0.001%
27	3.821	1001	1005	1010	rBV3	381	413	0.003%	0.004%
28	3.899	1022	1029	1032	rBV3	418	455	0.003%	0.005%
29	3.940	1037	1042	1045	rBV2	309	245	0.002%	0.003%
30	3.989	1055	1057	1059	rBV	313	187	0.001%	0.002%
31	4.056	1073	1078	1084	rBV2	183	251	0.002%	0.003%
32	4.120	1094	1098	1100	rBV2	259	238	0.002%	0.002%
33	4.175	1101	1115	1137	rBV2	74849	201277	13.00%	2.075%
34	4.436	1193	1196	1198	rBV	442	339	0.002%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081018\
 Data File : VU026050.D
 Acq On : 10 Aug 2018 17:57
 Operator : MD/SY
 Sample : J4361-24DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

35	4.493	1209	1214	1217	rBV2	467	493	0.03%	0.005%
36	4.564	1233	1236	1237	rBV	243	121	0.01%	0.001%
37	4.583	1240	1242	1243	rBV	222	85	0.01%	0.001%
38	4.648	1244	1262	1284	rBV	169493	400637	25.88%	4.129%
39	4.915	1343	1345	1347	rBV	313	145	0.01%	0.001%
40	5.021	1376	1378	1379	rBV	153	46	0.00%	0.000%
41	5.114	1404	1407	1411	rVB2	296	269	0.02%	0.003%
42	5.133	1411	1413	1416	rBV	181	95	0.01%	0.001%
43	5.149	1416	1418	1420	rBV	179	85	0.01%	0.001%
44	5.162	1420	1422	1424	rBV2	262	128	0.01%	0.001%
45	5.342	1451	1478	1501	rBV2	330201	976824	63.11%	10.068%
46	5.513	1529	1531	1534	rVB2	361	168	0.01%	0.002%
47	5.587	1552	1554	1557	rBV	571	366	0.02%	0.004%
48	5.619	1561	1564	1567	rVB2	206	147	0.01%	0.002%
49	5.635	1567	1569	1575	rBV	440	421	0.03%	0.004%
50	5.773	1610	1612	1614	rBV	128	47	0.00%	0.000%
51	5.889	1634	1648	1669	rBV	355967	696008	44.97%	7.174%
52	6.101	1709	1714	1716	rBV2	391	317	0.02%	0.003%
53	6.143	1723	1727	1729	rBV2	284	213	0.01%	0.002%
54	6.159	1729	1732	1735	rVV2	272	249	0.02%	0.003%
55	6.236	1755	1756	1757	rBV	298	66	0.00%	0.001%
56	6.268	1762	1766	1768	rBV2	375	293	0.02%	0.003%
57	6.333	1772	1786	1809	rBV	219493	438056	28.30%	4.515%
58	6.432	1814	1817	1818	rBV2	387	163	0.01%	0.002%
59	6.445	1818	1821	1822	rBV	267	133	0.01%	0.001%
60	6.529	1844	1847	1848	rBV	343	207	0.01%	0.002%
61	6.673	1887	1892	1894	rBV2	343	280	0.02%	0.003%
62	6.767	1915	1921	1922	rBV2	269	248	0.02%	0.003%
63	6.815	1932	1936	1941	rBV2	326	383	0.02%	0.004%
64	6.937	1967	1974	1980	rBV4	732	934	0.06%	0.010%
65	6.982	1986	1988	1992	rBV2	261	205	0.01%	0.002%
66	7.066	2012	2014	2016	rBV	119	56	0.00%	0.001%
67	7.095	2016	2023	2025	rBV3	409	442	0.03%	0.005%
68	7.230	2053	2065	2088	rBV	125495	220530	14.25%	2.273%
69	7.368	2103	2108	2110	rBV3	398	307	0.02%	0.003%
70	7.455	2132	2135	2136	rBV2	376	201	0.01%	0.002%
71	7.567	2150	2170	2187	rBV	460148	792978	51.23%	8.173%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081018\
 Data File : VU026050.D
 Acq On : 10 Aug 2018 17:57
 Operator : MD/SY
 Sample : J4361-24DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Title : VOC Analysis

72	7.760	2226	2230	2232	rBV	380	291	0.02%	0.003%
73	7.850	2248	2258	2278	rBV	87792	147825	9.55%	1.524%
74	8.181	2349	2361	2374	rBV	53173	124368	8.03%	1.282%
75	8.313	2394	2402	2432	rVB	248083	421935	27.26%	4.349%
76	8.818	2556	2559	2562	rBV3	363	284	0.02%	0.003%
77	9.091	2631	2644	2648	rBV	528602	815139	52.66%	8.402%
78	9.326	2713	2717	2721	rBV	523	630	0.04%	0.006%
79	9.384	2732	2735	2740	rVB2	532	368	0.02%	0.004%
80	9.439	2748	2752	2756	rBV	433	422	0.03%	0.004%
81	9.471	2758	2762	2766	rVB3	480	472	0.03%	0.005%
82	9.979	2916	2920	2924	rBV	431	395	0.03%	0.004%
83	10.062	2943	2946	2949	rBV	438	353	0.02%	0.004%
84	10.104	2953	2959	2960	rBV2	477	489	0.03%	0.005%
85	10.435	3049	3062	3080	rBV	293010	467578	30.21%	4.819%
86	10.615	3109	3118	3130	rVB5	13869	24824	1.60%	0.256%
87	10.811	3175	3179	3187	rBV3	422	697	0.05%	0.007%
88	10.876	3197	3199	3202	rBV	385	287	0.02%	0.003%
89	11.075	3259	3261	3263	rBV2	342	208	0.01%	0.002%
90	11.313	3329	3335	3341	rBV3	530	787	0.05%	0.008%
91	11.419	3358	3368	3378	rBV	51771	79532	5.14%	0.820%
92	11.487	3378	3389	3392	rBV	536920	771185	49.82%	7.949%
93	11.618	3428	3430	3433	rBV3	482	284	0.02%	0.003%
94	11.876	3494	3510	3526	rBV2	665841	1547845	100.00%	15.954%
95	12.442	3683	3686	3690	rBV2	509	499	0.03%	0.005%
96	13.506	4005	4017	4045	rBV	311903	511770	33.06%	5.275%
97	13.991	4158	4168	4189	rBV2	72958	121376	7.84%	1.251%


Sum of corrected areas: 9702037

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081018\
Data File : VU026050.D
Acq On : 10 Aug 2018 17:57
Operator : MD/SY
Sample : J4361-24DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

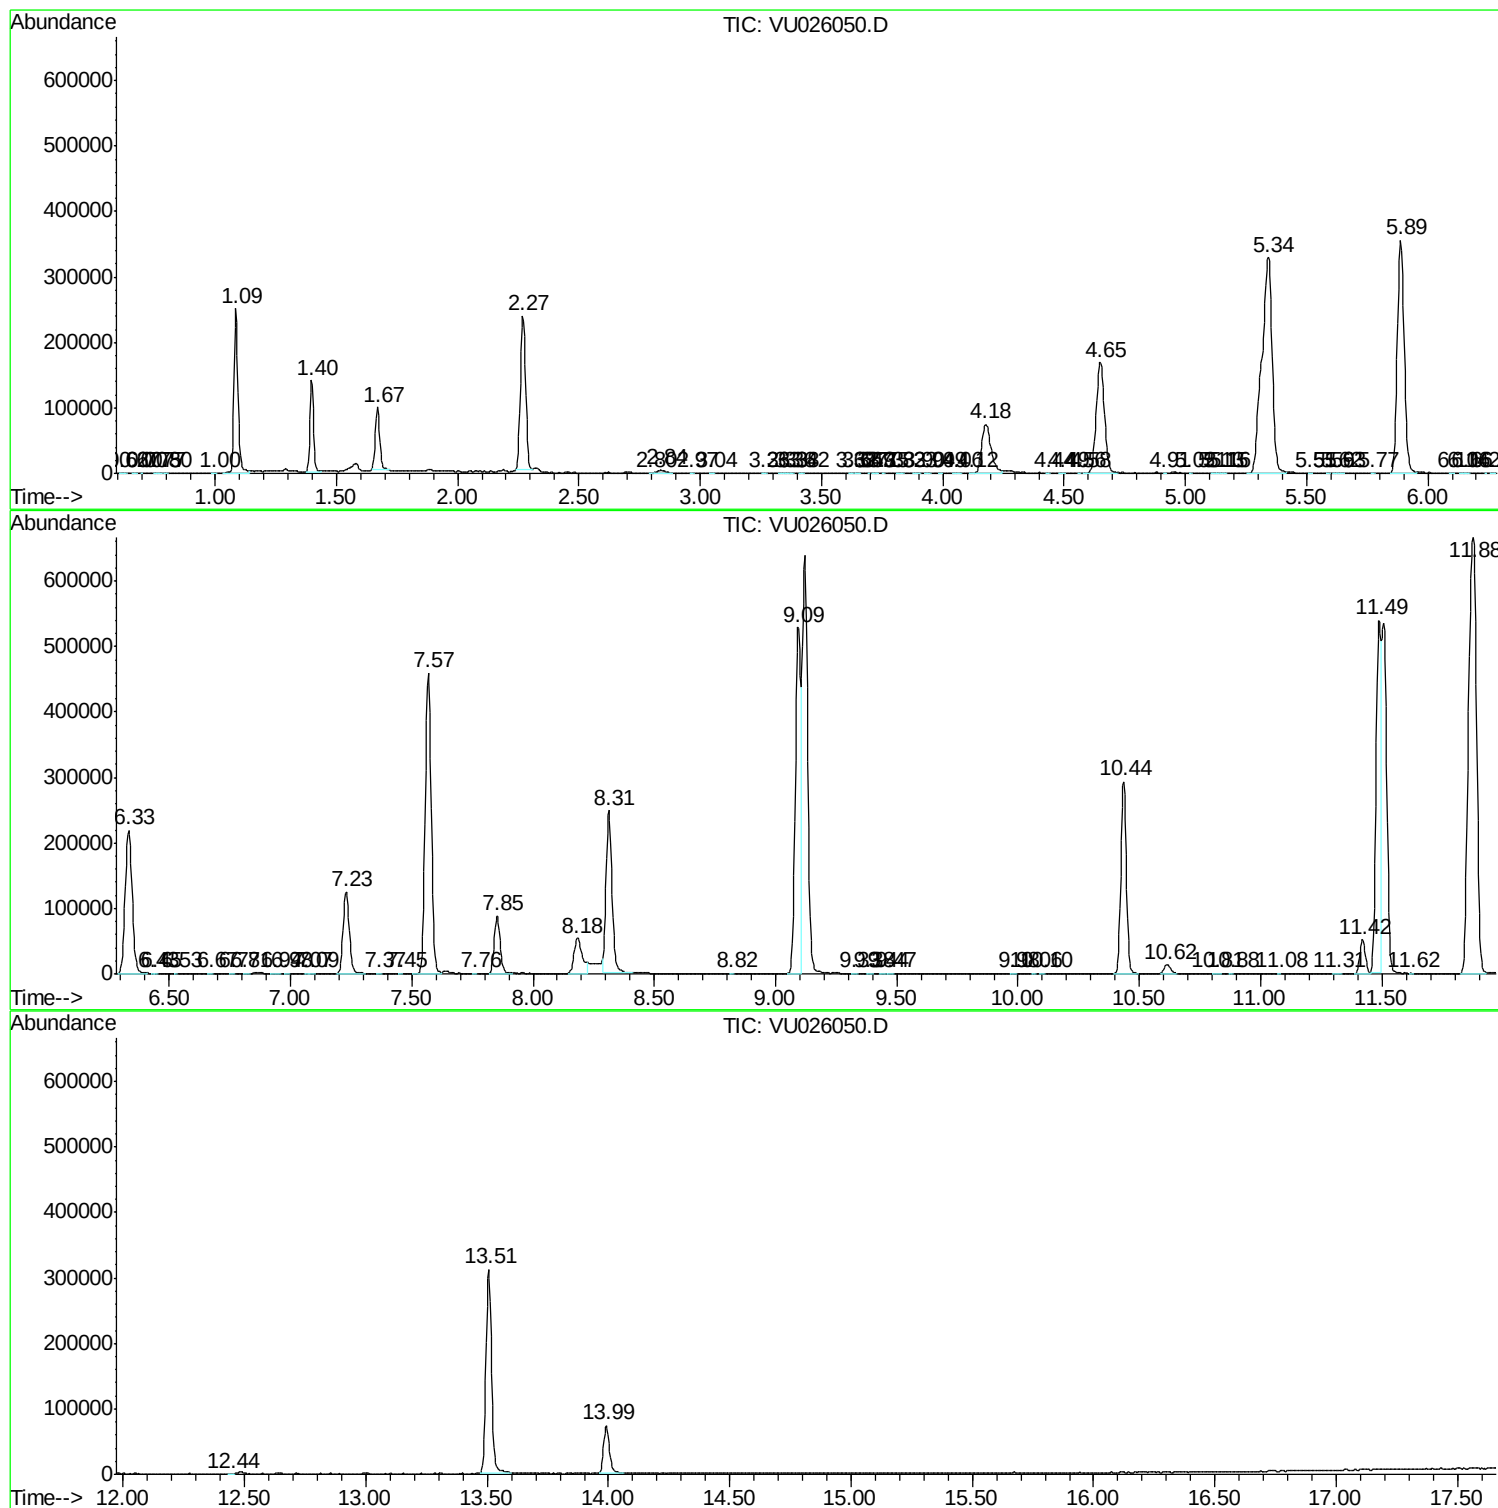

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU081018\
Data File : VU026050.D
Acq On : 10 Aug 2018 17:57
Operator : MD/SY
Sample : J4361-24DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU081018\
Data File : VU026050.D
Acq On : 10 Aug 2018 17:57
Operator : MD/SY
Sample : J4361-24DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc