


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081018\
Data File : VU026034.D
Acq On : 10 Aug 2018 09:33
Operator : MD/SY
Sample : BFB44
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Title : VOC Analysis
Last Update : Sat Aug 11 00:58:27 2018

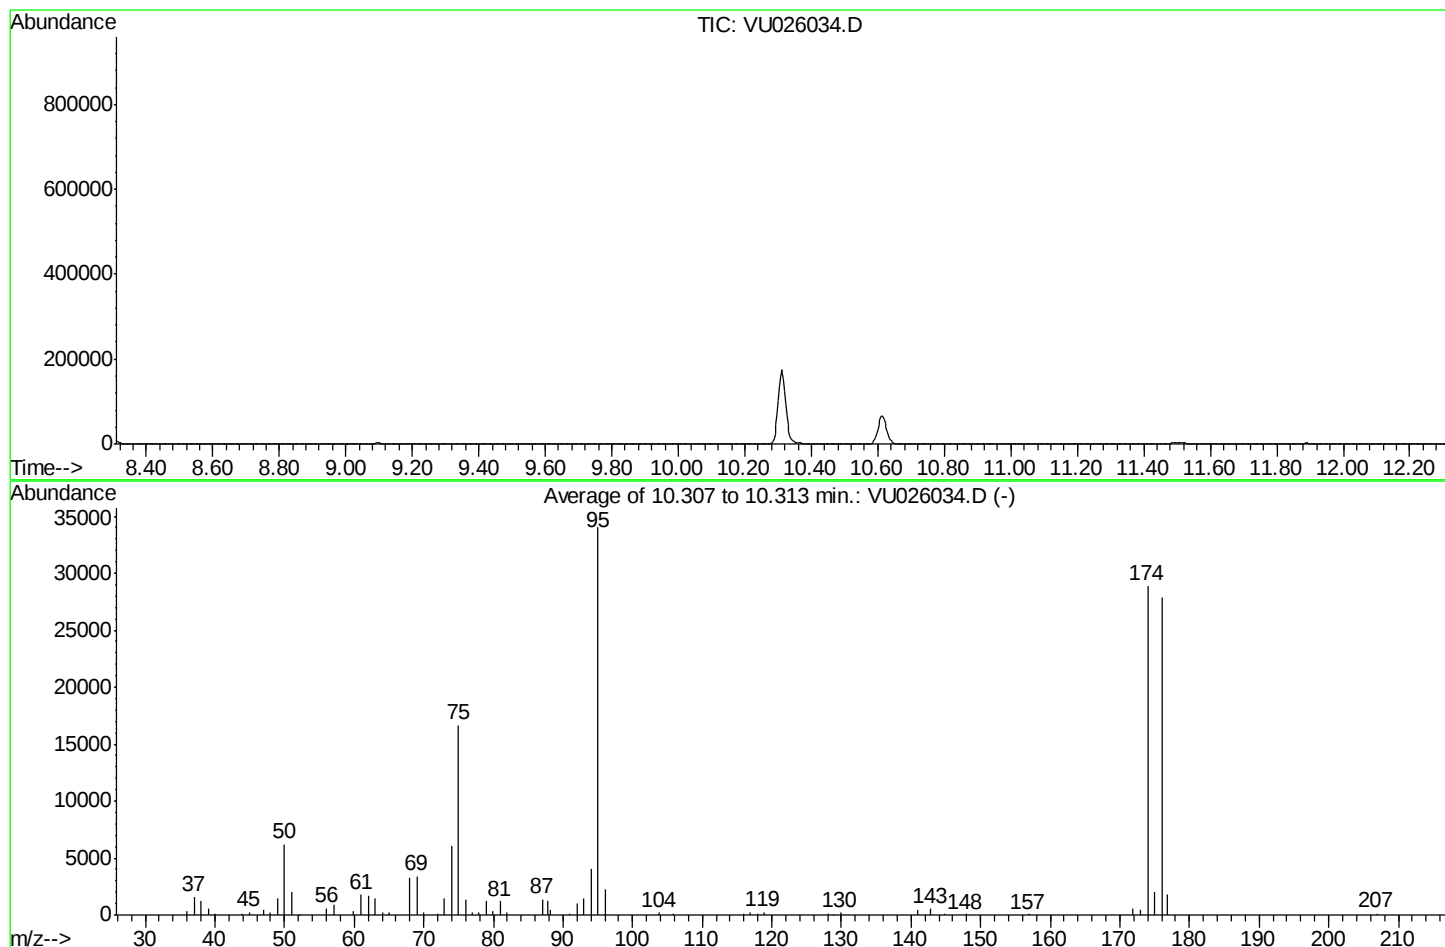

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	6184	PASS
75	95	30	80	49.0	16685	PASS
95	95	100	100	100.0	34032	PASS
96	95	5	9	6.6	2237	PASS
173	174	0.00	2	1.4	400	PASS
174	95	50	120	85.0	28936	PASS
175	174	5	9	7.0	2026	PASS
176	174	95	101	96.3	27856	PASS
177	176	5	9	6.4	1773	PASS

Scan 3011 (10.271 min): VU026034.D
BFB44

m/z	Abundance
43.90	415.0
281.10	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	337.0
37.00	1528.0
38.00	1172.0
39.00	577.0
40.00	111.0
43.90	493.0
45.00	272.0
47.00	381.0
47.90	272.0
49.00	1498.0
50.00	6266.0
51.00	1965.0
56.10	537.0
57.00	973.0
59.90	395.0
61.00	1630.0
62.00	1625.0
63.00	1374.0
64.10	166.0
65.10	193.0
68.00	3286.0
69.00	3193.0
69.90	253.0
72.00	149.0
73.00	1424.0
74.00	5783.0
75.00	16424.0
76.00	1326.0
77.00	270.0
77.90	169.0
78.90	1281.0
80.00	371.0
80.90	1165.0
81.80	298.0
87.00	1365.0
87.90	1080.0
90.90	168.0
92.00	1079.0
93.00	1381.0
94.00	3788.0
95.00	32248.0
96.00	2168.0
103.90	164.0
105.80	182.0
115.90	133.0
116.80	192.0
118.00	116.0
118.80	188.0
129.90	165.0
140.90	461.0
142.90	485.0
147.90	109.0
171.90	479.0
172.90	412.0
174.00	27600.0
175.00	1984.0
176.00	26280.0
176.90	1693.0
206.80	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.90	318.0
37.00	1658.0
38.00	1265.0
39.00	568.0
40.00	117.0
44.00	516.0
44.90	287.0
47.00	473.0
48.00	291.0
49.00	1587.0
50.00	6318.0
51.00	2054.0
52.10	109.0
56.00	582.0
57.00	934.0
59.90	406.0
61.00	1872.0
62.00	1684.0
63.00	1566.0
64.10	203.0
65.00	230.0
68.00	3308.0
69.00	3503.0
69.90	249.0
72.00	172.0
73.00	1461.0
74.00	6374.0
75.00	17096.0
76.00	1425.0
77.00	311.0
77.90	232.0
78.90	1301.0
79.90	373.0
81.00	1206.0
81.80	282.0
87.00	1426.0
87.90	1213.0
88.10	1208.0
90.90	171.0
92.00	1030.0
93.00	1478.0
94.00	4219.0
95.00	35112.0
96.00	2307.0
103.90	189.0
105.80	166.0
115.90	159.0
116.90	192.0
118.00	146.0
118.80	259.0
128.00	100.0
129.90	204.0
140.90	409.0
142.90	556.0
144.90	101.0
147.80	111.0
156.90	117.0
171.90	553.0
172.90	426.0
174.00	29736.0
175.00	2072.0
176.00	28712.0
176.90	1818.0
206.90	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
35.00	243.0
37.00	1562.0
38.00	1215.0
39.00	540.0
40.10	141.0
44.00	511.0
44.90	269.0
47.10	487.0
48.00	281.0
49.00	1469.0
50.00	5968.0
51.00	1928.0
56.00	620.0
57.10	875.0
60.00	365.0
61.00	1852.0
62.00	1596.0
63.00	1566.0
64.10	186.0
65.00	249.0
68.00	3110.0
69.00	3458.0
69.90	224.0
72.00	155.0
73.00	1436.0
74.00	6222.0
75.00	16536.0
76.00	1385.0
77.00	266.0
77.90	229.0
78.90	1302.0
79.90	317.0
81.00	1182.0
81.90	253.0
87.00	1275.0
87.90	1288.0
90.90	143.0
92.00	961.0
93.00	1602.0
94.00	4238.0
95.00	34736.0
96.00	2238.0
103.90	182.0
105.80	136.0
116.00	154.0
116.90	197.0
117.90	155.0
118.90	277.0
128.00	121.0
128.80	101.0
129.90	211.0
140.90	349.0
142.80	544.0
144.90	149.0
147.80	112.0
156.90	134.0
171.90	536.0
173.00	364.0
174.00	29472.0
175.00	2023.0
176.00	28576.0
176.90	1810.0
207.00	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44