


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081019\
 Data File : VU033718.D
 Acq On : 10 Aug 2019 09:20
 Operator : JC/SP
 Sample : BFB52
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080919WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 12 18:44:30 2019

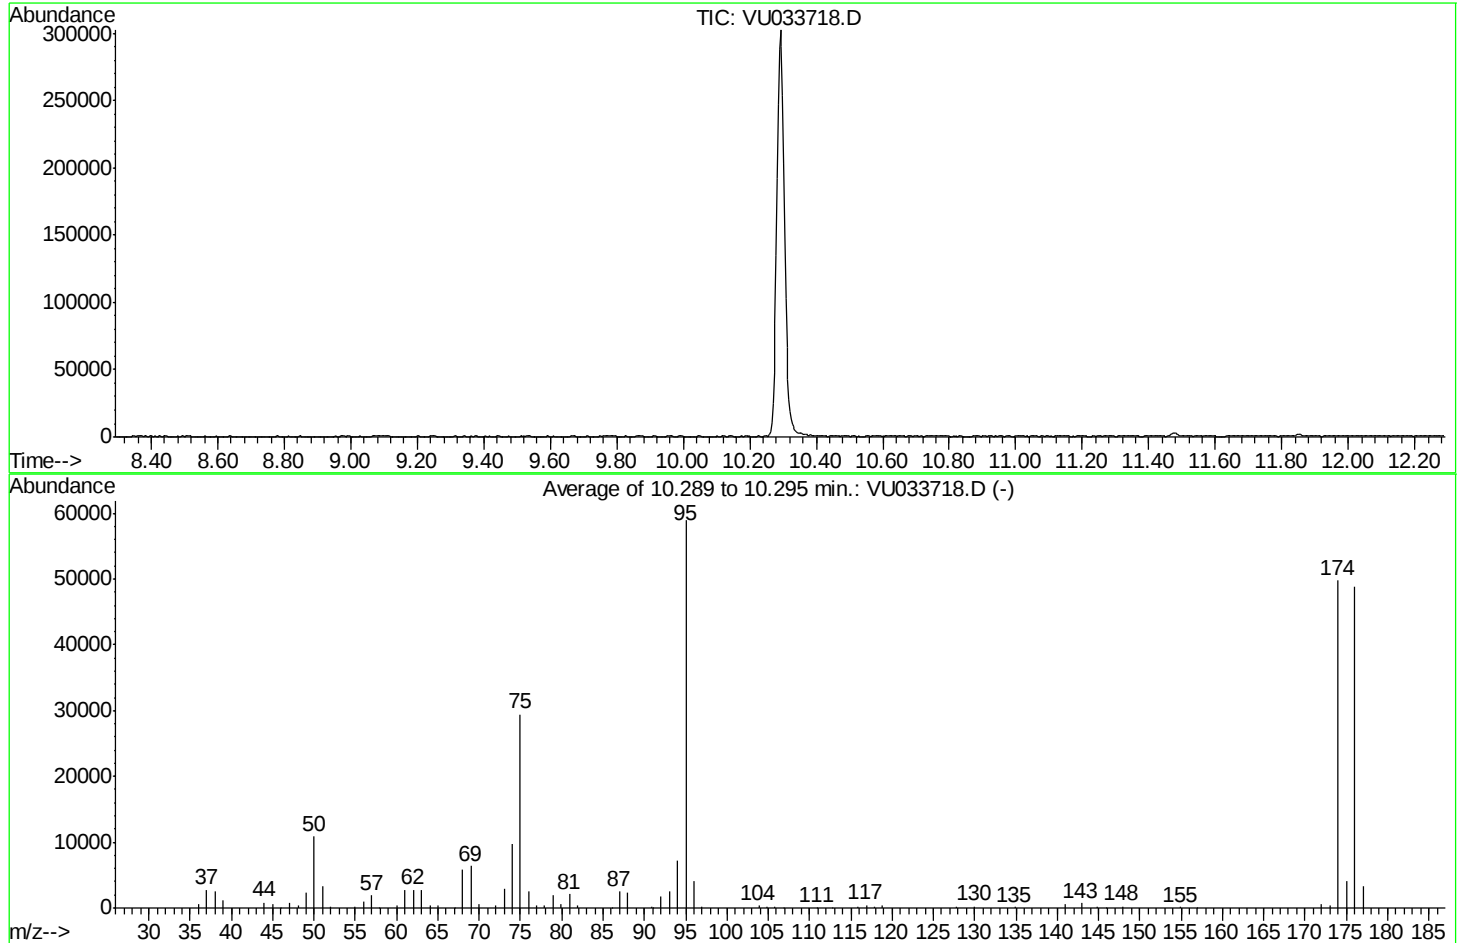

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	10886	PASS
75	95	30	80	49.9	29392	PASS
95	95	100	100	100.0	58912	PASS
96	95	5	9	6.9	4069	PASS
173	174	0.00	2	0.6	313	PASS
174	95	50	120	84.4	49712	PASS
175	174	5	9	8.3	4140	PASS
176	174	95	101	98.1	48760	PASS
177	176	5	9	6.8	3307	PASS

m/z	Abundance
36.00	635.0
37.00	2729.0
38.00	2618.0
39.00	1057.0
39.90	140.0
43.90	718.0
45.00	502.0
46.00	115.0
46.90	860.0
48.00	377.0
49.00	2523.0
50.00	10756.0
51.00	3335.0
52.00	158.0
55.00	141.0
56.00	916.0
57.00	1903.0
57.90	124.0
60.10	504.0
61.00	2692.0
62.00	2851.0
63.00	2565.0
64.00	290.0
65.00	364.0
68.00	5832.0
69.00	6340.0
70.00	593.0
72.00	325.0
73.00	2840.0
74.00	9755.0
75.00	29160.0
76.00	2671.0
76.90	348.0
77.90	381.0
78.90	1961.0
80.00	493.0
80.90	2088.0
81.90	469.0
86.10	146.0
87.00	2468.0
88.00	2402.0
90.80	186.0
91.10	184.0
92.00	1604.0
93.00	2659.0
94.00	7116.0
95.00	58344.0
96.00	4042.0
97.00	102.0
103.90	281.0
104.80	125.0
105.80	225.0
110.90	120.0
115.90	204.0
116.90	370.0
117.90	258.0
118.80	338.0
127.80	217.0
130.00	191.0
134.90	113.0
140.90	561.0
143.00	668.0
144.90	244.0
145.90	110.0
147.90	170.0
154.90	148.0
171.90	529.0
174.00	47528.0
175.00	4019.0
176.00	46720.0
177.00	3198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
40.00	184.0
44.20	326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	533.0
37.00	2817.0
38.00	2475.0
39.00	1122.0
39.90	164.0
44.00	852.0
45.00	557.0
47.00	743.0
48.10	405.0
49.00	2155.0
50.00	10641.0
51.00	3362.0
52.10	108.0
54.90	127.0
56.00	827.0
57.00	1778.0
60.00	435.0
61.00	2699.0
62.00	2712.0
63.00	2702.0
64.00	318.0
65.00	418.0
67.00	133.0
68.00	5835.0
69.00	6119.0
70.00	483.0
72.00	326.0
73.00	2807.0
74.00	9440.0
75.00	28760.0
76.00	2192.0
77.00	321.0
77.90	238.0
78.90	2033.0
79.90	542.0
80.90	2080.0
81.90	294.0
87.00	2452.0
88.00	2185.0
90.90	179.0
92.00	1688.0
93.00	2478.0
94.00	6827.0
95.00	57512.0
96.00	3982.0
96.90	124.0
103.80	313.0
104.80	105.0
105.90	298.0
106.90	104.0
112.70	109.0
115.80	175.0
116.90	456.0
117.80	263.0
118.80	370.0
127.70	166.0
130.00	187.0
134.90	156.0
140.90	498.0
142.90	745.0
144.90	211.0
147.90	204.0
155.00	132.0
156.90	130.0
171.90	693.0
173.00	939.0
174.00	50440.0
175.00	4110.0
176.00	49216.0
177.00	3306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	619.0
37.00	2911.0
38.00	2727.0
39.00	1139.0
39.90	142.0
44.00	848.0
45.10	548.0
47.00	833.0
48.00	398.0
49.00	2517.0
50.00	11262.0
51.00	3452.0
52.00	150.0
54.90	138.0
56.00	947.0
57.00	1967.0
57.90	131.0
60.10	491.0
61.00	2796.0
62.00	2890.0
63.00	2723.0
64.00	302.0
64.90	437.0
67.10	151.0
68.00	6064.0
69.00	6545.0
70.00	563.0
72.00	333.0
73.00	3047.0
74.00	9863.0
75.00	30256.0
76.00	2542.0
76.90	332.0
77.90	324.0
78.90	2064.0
79.90	534.0
80.90	2146.0
81.90	378.0
86.10	139.0
87.00	2534.0
88.00	2534.0
90.80	174.0
92.00	1746.0
93.00	2734.0
94.00	7456.0
95.00	60880.0
96.00	4184.0
96.90	135.0
103.80	301.0
104.80	122.0
105.90	265.0
110.90	126.0
115.90	188.0
116.90	432.0
117.80	268.0
118.80	353.0
127.80	187.0
130.00	211.0
134.90	128.0
140.90	563.0
143.00	736.0
144.90	248.0
147.90	217.0
154.90	153.0
171.90	614.0
174.00	51168.0
175.00	4293.0
176.00	50344.0
177.00	3419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52