

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081020\
 Data File : VU039827.D
 Acq On : 10 Aug 2020 16:23
 Operator : SY/MD
 Sample : VIBLK46
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK46

Quant Time: Aug 11 05:37:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 11 04:57:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	73506	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	73522	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	35975	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	23447	5.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.20%
7) Chloroethane-d5	1.92	69	21987	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.58	63	33251	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.20%
20) 2-Butanone-d5	4.66	46	85315	48.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.74%
24) Chloroform-d	5.08	84	41962	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
26) 1,2-Dichloroethane-d4	5.72	65	26915	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.75	84	87151	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.70	67	28201	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.91	98	71779	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	8.19	79	10380	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.64	63	60477	48.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.32%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	25821	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	33113	5.38	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.60%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	1499	0.212 ug/L	90
25) Chloroform	5.11	83	4937	0.510 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081020\
Data File : VU039827.D
Acq On : 10 Aug 2020 16:23
Operator : SY/MD
Sample : VIBLK46
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK46

Quant Time: Aug 11 05:37:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 11 04:57:12 2020
Response via : Initial Calibration




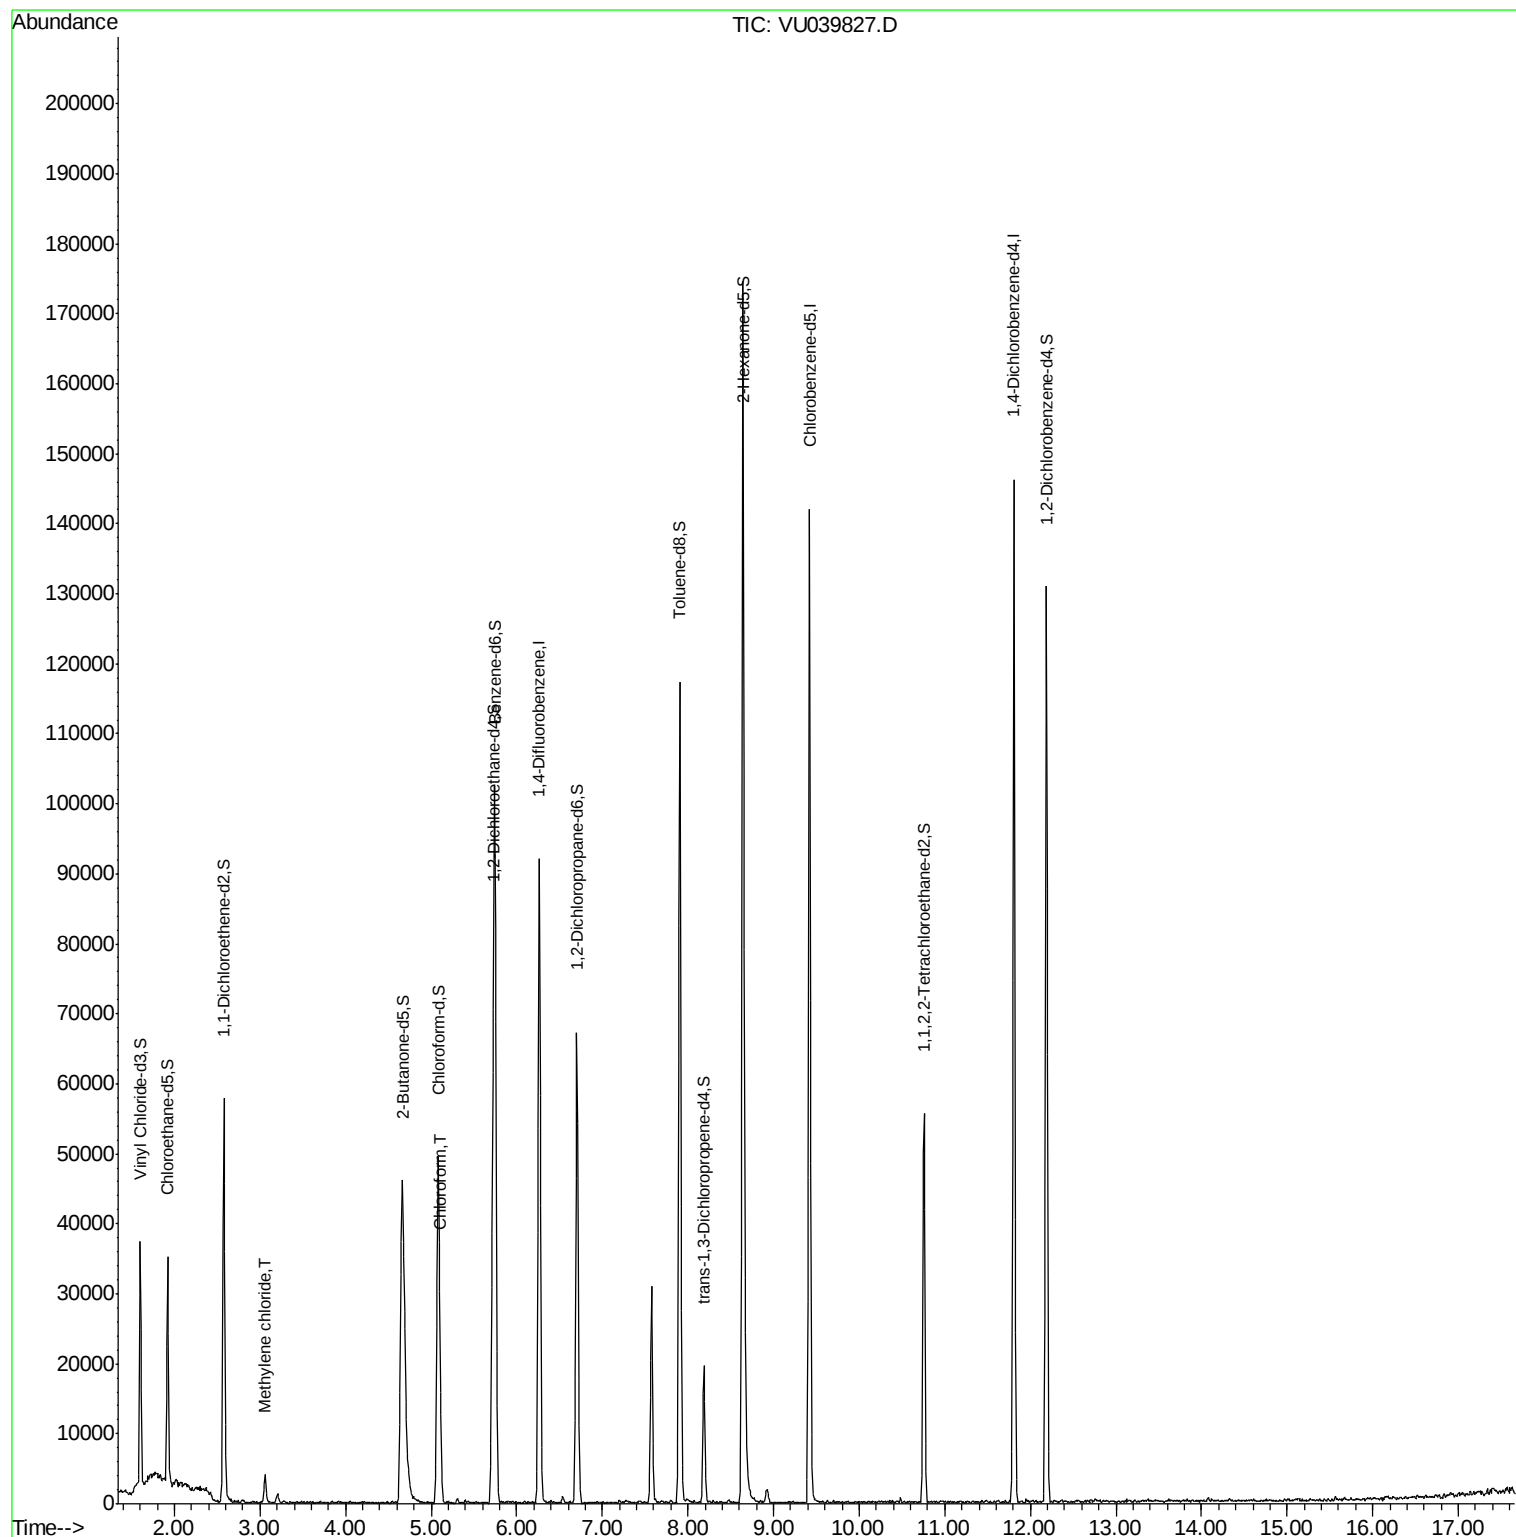


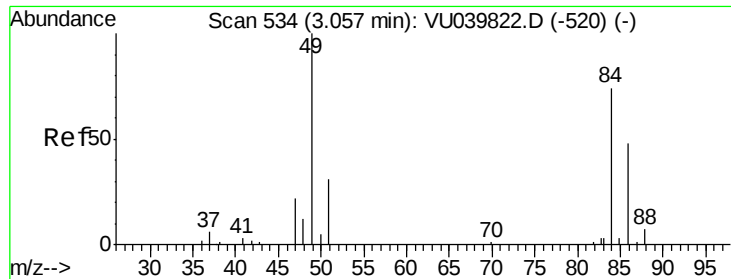

#16
Methvlene chloride
Concen: 0.212 ug/L
RT: 3.06 min Scan# 535
Delta R.T. 0.00 min
Lab File: VU039827.D
Acq: 10 Aug 2020 16:23

Instrument :
MSVOA_U
ClientSampleId :
VIBLK46

Tot Ion: 84 Resp: 1499
Ion Ratio Lower Upper
84 100
86 68.5 43.9 81.5
49 122.3 94.4 175.4

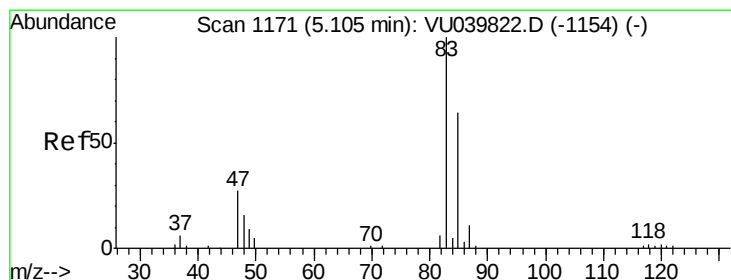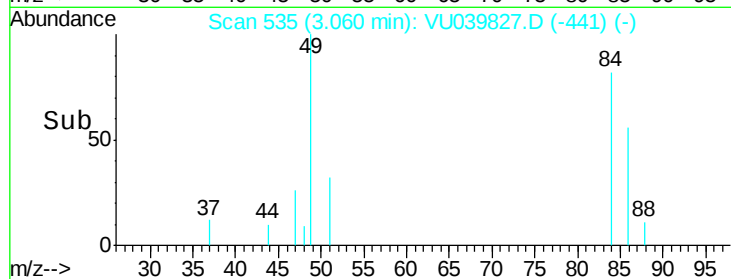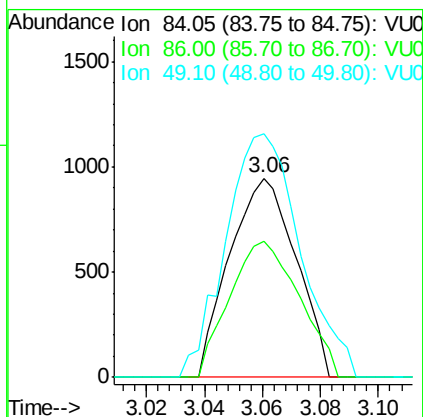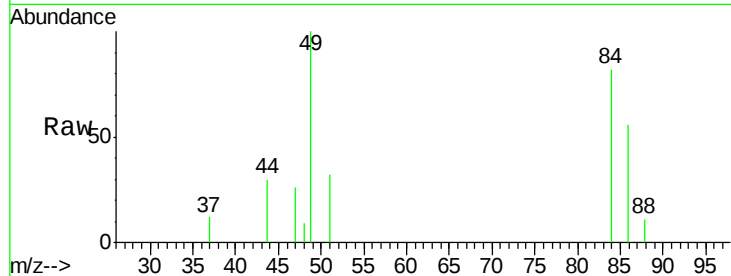

#25
Chloroform
Concen: 0.510 ug/L
RT: 5.11 min Scan# 1172
Delta R.T. 0.00 min
Lab File: VU039827.D
Acq: 10 Aug 2020 16:23

Tgt Ion: 83 Resp: 4937
Ion Ratio Lower Upper
83 100
85 69.7 42.1 78.3

