


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081020\
 Data File : VU039821.D
 Acq On : 10 Aug 2020 08:59
 Operator : SY/MD
 Sample : BFB12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 11 01:16:25 2020

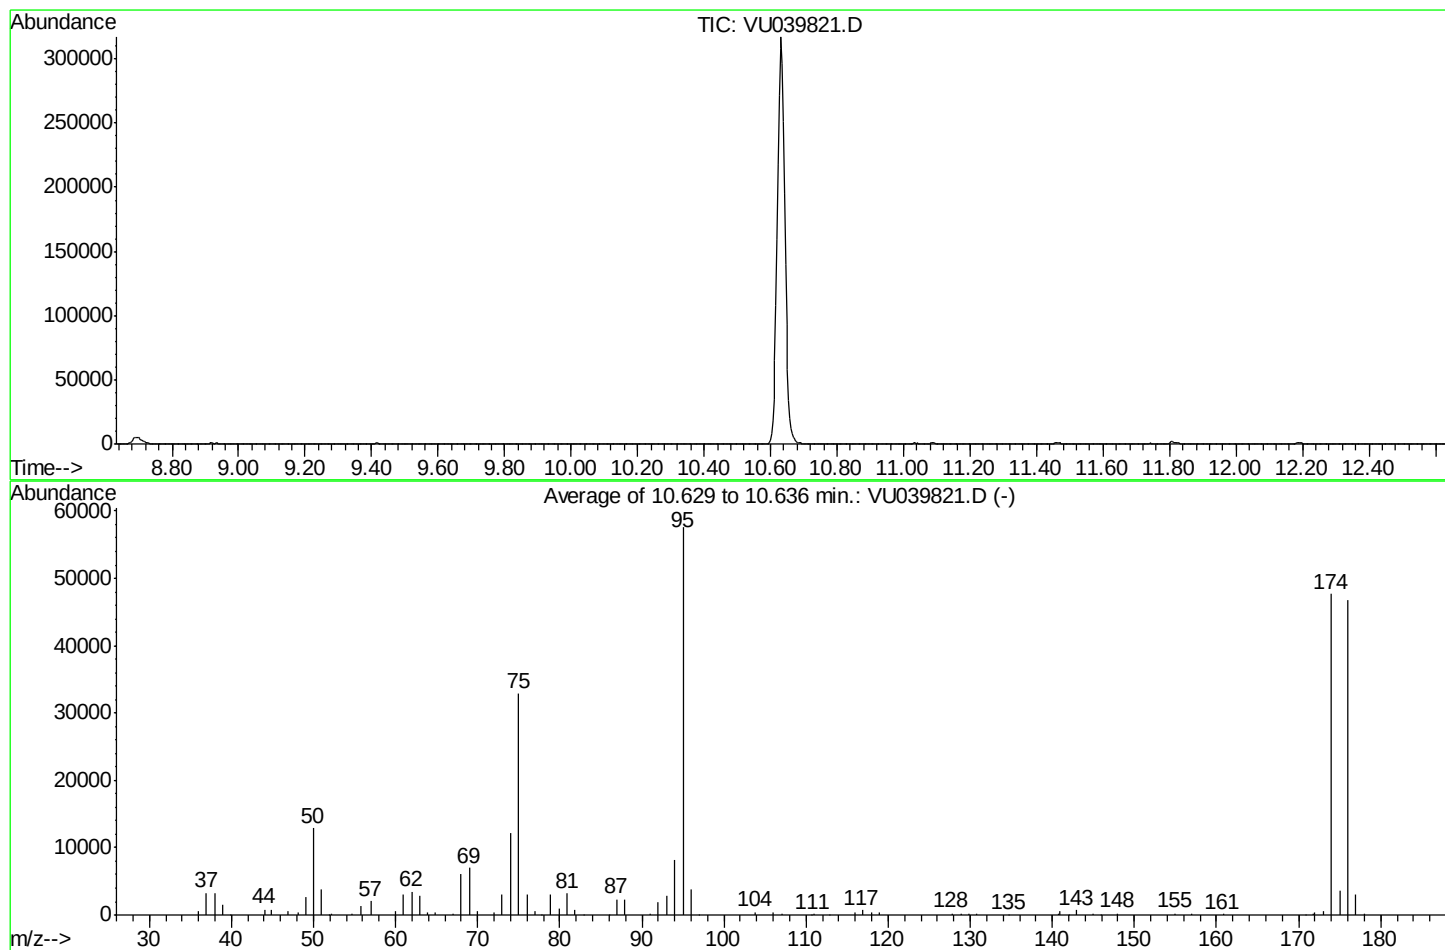

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	12903	PASS
75	95	30	80	57.0	32840	PASS
95	95	100	100	100.0	57576	PASS
96	95	5	9	6.6	3821	PASS
173	174	0.00	2	1.4	668	PASS
174	95	50	120	82.8	47674	PASS
175	174	5	9	7.6	3640	PASS
176	174	95	101	98.0	46730	PASS
177	176	5	9	6.4	2998	PASS

m/z	Abundance
39.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	545.0
36.90	3286.0
38.00	3177.0
39.00	1563.0
39.80	152.0
44.10	716.0
44.90	730.0
46.90	642.0
48.10	423.0
49.00	2787.0
50.00	13033.0
50.90	3812.0
52.10	141.0
54.80	282.0
55.80	1225.0
57.00	2223.0
60.00	463.0
61.00	3243.0
62.00	3493.0
63.00	2901.0
63.80	378.0
64.90	345.0
67.00	218.0
67.90	6339.0
69.00	7257.0
69.90	537.0
71.90	305.0
73.00	3037.0
74.00	12511.0
75.00	32984.0
76.00	3187.0
77.00	523.0
78.90	3337.0
79.90	1069.0
80.90	3095.0
81.80	699.0
86.90	2234.0
87.80	2194.0
91.00	233.0
91.90	1998.0
93.00	2910.0
94.00	8430.0
95.00	58312.0
96.00	4012.0
103.80	437.0
105.90	408.0
107.10	113.0
111.00	204.0
112.90	161.0
115.80	322.0
116.90	622.0
118.00	366.0
118.90	485.0
127.80	170.0
128.90	119.0
129.90	165.0
130.90	158.0
134.70	109.0
140.80	752.0
142.90	789.0
145.00	197.0
147.90	207.0
154.90	171.0
157.00	170.0
160.80	117.0
170.80	101.0
171.80	728.0
173.00	609.0
174.00	46856.0
175.00	3870.0
176.00	45984.0
177.00	2928.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	658.0
37.00	3349.0
38.00	3303.0
39.00	1488.0
39.80	204.0
44.00	820.0
44.90	781.0
46.90	600.0
48.10	396.0
49.00	2759.0
50.00	13381.0
51.00	3895.0
51.80	127.0
52.20	130.0
54.70	313.0
55.80	1314.0
57.00	2106.0
59.90	484.0
61.00	3145.0
62.00	3565.0
63.00	3008.0
63.90	453.0
64.80	332.0
67.00	226.0
68.00	6310.0
69.00	7299.0
70.00	577.0
72.00	290.0
73.00	3147.0
74.00	12628.0
75.00	33720.0
76.00	3126.0
77.10	517.0
78.90	3177.0
79.90	1067.0
80.90	3311.0
81.80	820.0
82.90	108.0
86.00	119.0
86.90	2419.0
87.90	2331.0
91.00	255.0
91.90	2033.0
93.00	2878.0
94.00	8368.0
95.00	59416.0
96.00	3957.0
96.90	111.0
103.80	462.0
105.90	408.0
107.10	137.0
110.90	152.0
112.90	143.0
115.90	307.0
116.90	701.0
118.00	320.0
118.90	478.0
127.80	202.0
128.90	172.0
129.90	178.0
130.80	152.0
141.00	826.0
142.00	104.0
142.90	723.0
144.90	182.0
145.80	100.0
148.00	221.0
154.90	218.0
157.00	177.0
160.80	147.0
170.90	117.0
172.00	696.0
173.00	706.0
174.00	49064.0
175.00	3742.0
176.00	48176.0
177.00	3107.0
178.00	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	632.0
37.00	3087.0
38.00	3022.0
39.00	1256.0
39.90	188.0
44.00	875.0
44.90	695.0
46.90	528.0
48.10	343.0
49.00	2446.0
50.00	12295.0
51.00	3758.0
51.80	109.0
52.20	105.0
54.70	244.0
55.90	1236.0
57.00	1881.0
59.90	532.0
60.90	2806.0
62.00	3253.0
63.00	2686.0
63.90	427.0
64.80	277.0
67.00	240.0
68.00	5774.0
69.00	6491.0
70.00	637.0
71.80	264.0
72.10	269.0
73.00	2992.0
74.00	11653.0
75.00	31816.0
76.00	2737.0
77.10	428.0
77.80	249.0
78.90	2629.0
79.90	902.0
80.90	3168.0
81.90	803.0
82.90	124.0
86.00	102.0
86.90	2233.0
87.90	2091.0
91.00	282.0
91.90	1860.0
93.00	2692.0
94.00	7478.0
95.00	55000.0
96.00	3494.0
96.90	134.0
103.90	459.0
106.00	374.0
107.00	125.0
110.70	109.0
116.00	270.0
116.90	698.0
117.90	263.0
119.00	460.0
127.70	220.0
128.90	166.0
129.90	172.0
130.80	138.0
140.90	889.0
141.90	117.0
143.00	697.0
144.90	145.0
145.90	108.0
148.00	195.0
155.00	228.0
157.00	161.0
160.80	124.0
172.00	607.0
173.00	689.0
174.00	47104.0
175.00	3309.0
176.00	46032.0
177.00	2961.0
178.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12