

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081021\
 Data File : VU044412.D
 Acq On : 10 Aug 2021 15:00
 Operator : SY/MD
 Sample : M3344-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Aug 11 01:10:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 11 01:08:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	163037	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	162238	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	77535	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	49476	3.632	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.912	69	60142	5.143	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.800%
11) 1,1-Dichloroethene-d2	2.568	65	23676	4.126	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	4.642	46	162627	40.260	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.520%
24) Chloroform-d	5.070	84	119447	5.039	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.800%
26) 1,2-Dichloroethane-d4	5.710	65	64798	4.897	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	5.735	84	243666	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	6.697	67	76440	4.839	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.903	98	215466	4.735	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	8.185	79	21960	3.571	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.400%
46) 2-Hexanone-d5	8.642	63	149159	40.172	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.340%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	62939	4.456	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	12.198	152	84013	5.627	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.600%
Target Compounds						Qvalue
16) Methylene chloride	3.051	84	4783	0.335	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081021\
Data File : VU044412.D
Acq On : 10 Aug 2021 15:00
Operator : SY/MD
Sample : M3344-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Aug 11 01:10:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 11 01:08:01 2021
Response via : Initial Calibration

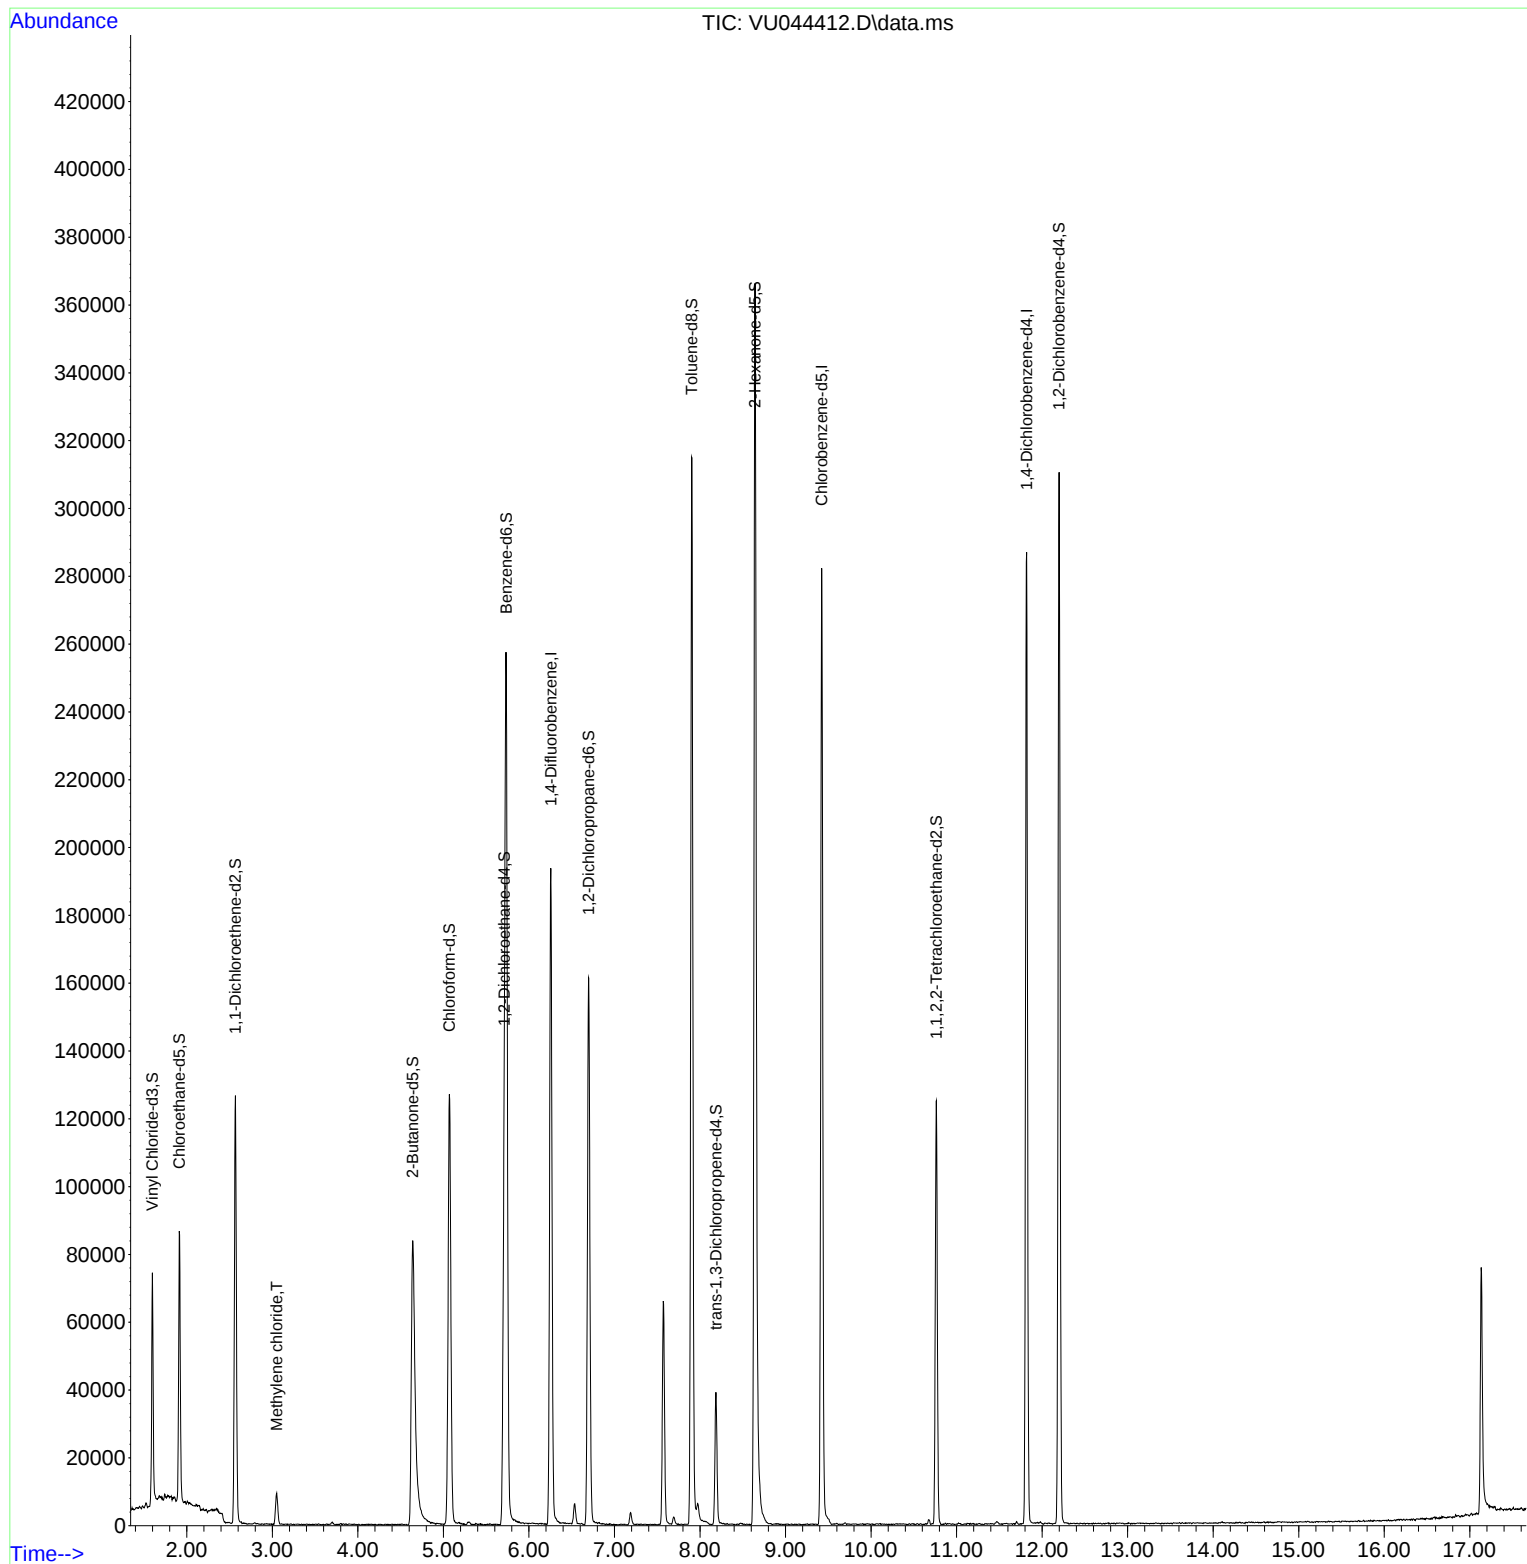

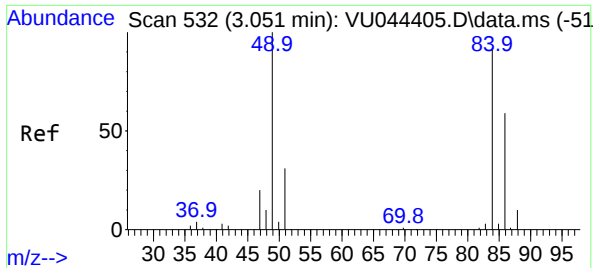

#16
Methylene chloride
Concen: 0.335 ug/L
RT: 3.051 min Scan# 532
Delta R.T. 0.000 min
Lab File: VU044412.D
Acq: 10 Aug 2021 15:00

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	4783
Ion	Ratio	Lower	Upper
84	100		
86	69.9	45.2	84.0
49	110.9	81.8	152.0

