
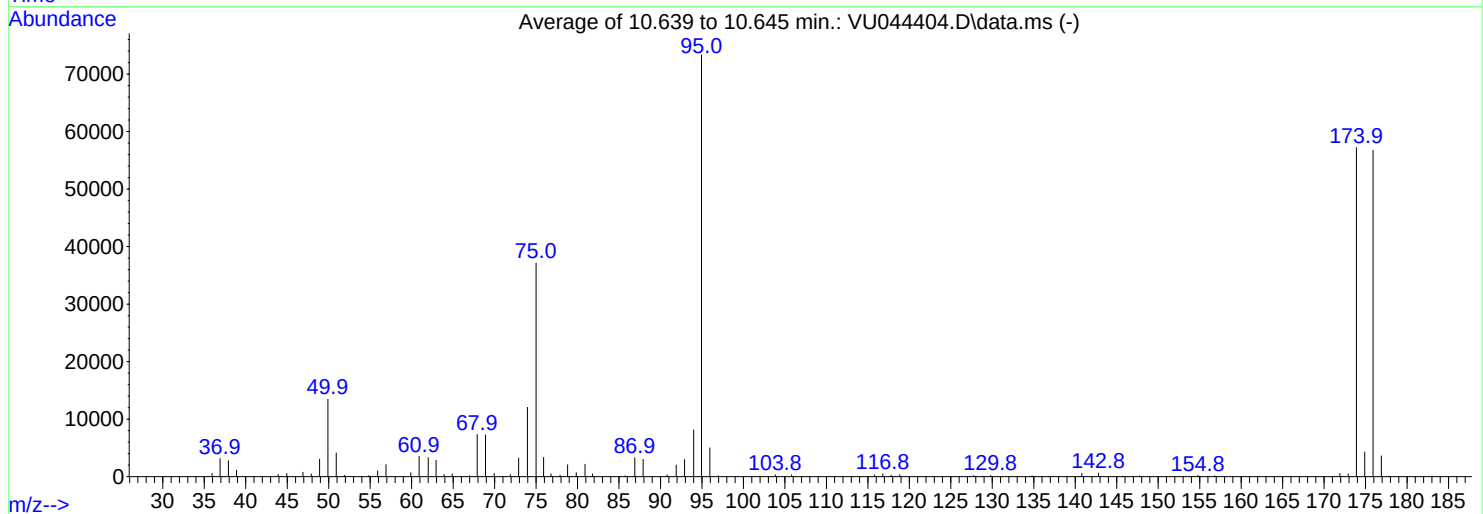


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081021\
Data File : VU044404.D
Acq On : 10 Aug 2021 09:09
Operator : SY/MD
Sample : BFB005
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB005

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072321WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Aug 11 01:08:01 2021

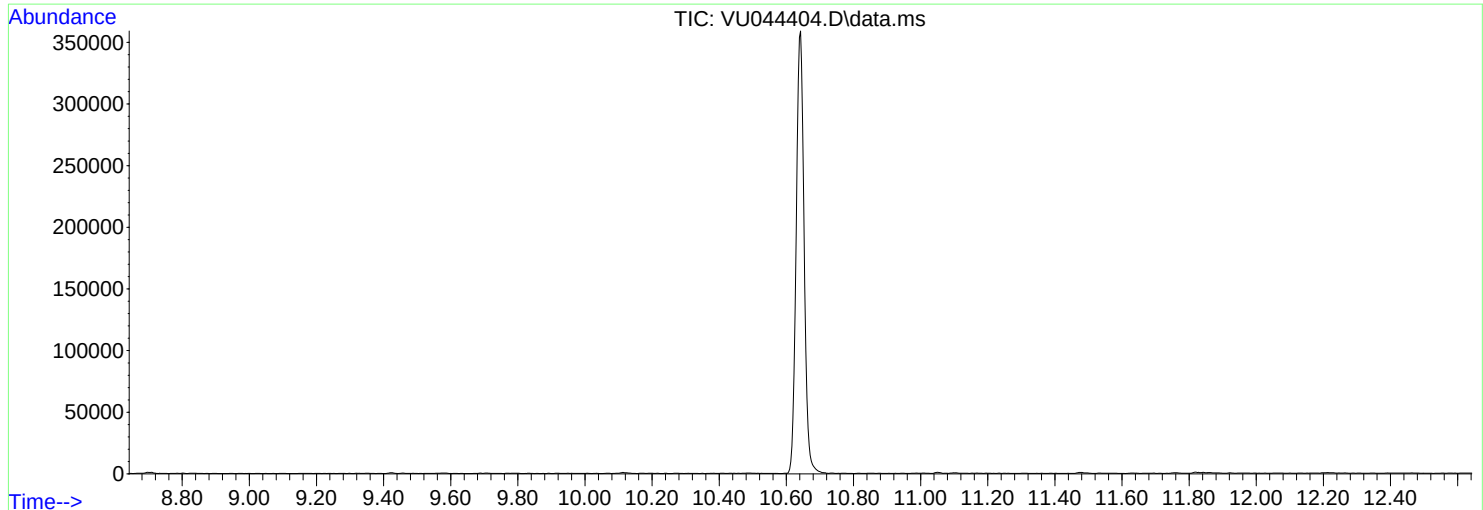

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	13457	PASS
75	95	30	80	50.6	37128	PASS
95	95	100	100	100.0	73344	PASS
96	95	5	9	6.8	5003	PASS
173	174	0.00	2	0.8	471	PASS
174	95	50	120	78.0	57195	PASS
175	174	5	9	7.5	4281	PASS
176	174	95	101	99.2	56723	PASS
177	176	5	9	6.4	3619	PASS

m/z	Abundance
36.00	539.0
36.90	2953.0
37.90	2512.0
38.90	1142.0
39.90	176.0
43.90	734.0
45.00	471.0
46.90	737.0
47.90	451.0
48.90	2848.0
49.90	12451.0
50.90	3959.0
51.90	199.0
54.80	157.0
55.90	1040.0
56.90	1917.0
59.90	668.0
60.90	3219.0
62.00	3006.0
63.00	2587.0
63.90	349.0
64.90	439.0
67.00	173.0
67.90	6950.0
68.90	6852.0
70.00	486.0
71.90	307.0
72.90	2957.0
73.90	11307.0
75.00	35408.0
75.90	3036.0
76.80	410.0
77.90	255.0
78.80	1936.0
79.80	654.0
80.90	1997.0
81.80	433.0
85.80	149.0
86.90	3215.0
87.90	2843.0
90.80	257.0
91.90	2016.0
92.90	2787.0
94.00	7768.0
95.00	69520.0
95.90	4741.0
96.90	150.0
103.80	307.0
105.80	292.0
115.80	237.0
116.80	414.0
117.80	240.0
118.80	298.0
127.80	197.0
129.80	260.0
134.80	134.0
136.80	103.0
140.80	552.0
142.80	589.0
147.70	131.0
154.80	201.0
156.80	141.0
171.90	480.0
172.90	451.0
173.90	55680.0
174.90	4133.0
175.90	55736.0
176.90	3537.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	558.0
36.90	3229.0
37.90	2842.0
38.90	1122.0
39.90	165.0
43.90	790.0
44.90	556.0
46.90	772.0
47.90	489.0
48.90	3136.0
49.90	13757.0
50.90	4259.0
51.90	228.0
54.90	183.0
55.90	1019.0
56.90	2144.0
59.90	713.0
60.90	3606.0
62.00	3427.0
63.00	2963.0
63.90	399.0
64.90	473.0
67.00	177.0
67.90	7545.0
68.90	7435.0
69.90	563.0
71.90	359.0
72.90	3309.0
74.00	12331.0
75.00	38296.0
75.90	3432.0
76.80	485.0
77.90	241.0
78.80	2108.0
79.80	702.0
80.90	2228.0
81.80	474.0
85.80	147.0
86.90	3412.0
87.90	3092.0
90.80	332.0
91.90	2029.0
92.90	3075.0
94.00	8404.0
94.90	75584.0
96.00	5178.0
96.90	185.0
103.80	299.0
105.80	305.0
115.80	285.0
116.80	502.0
117.80	257.0
118.80	337.0
127.70	219.0
128.80	118.0
129.80	271.0
134.80	138.0
140.80	568.0
142.80	644.0
145.70	111.0
147.70	130.0
154.80	223.0
156.80	159.0
171.90	566.0
172.90	478.0
173.90	58856.0
174.90	4412.0
175.90	58488.0
176.90	3748.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
39.90	116.0
43.90	375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
36.00	550.0
36.90	3239.0
37.90	2934.0
38.90	1097.0
39.90	181.0
43.90	791.0
44.90	616.0
46.90	741.0
47.90	476.0
48.90	3156.0
49.90	14164.0
50.90	4180.0
51.90	237.0
54.90	188.0
55.90	946.0
56.90	2186.0
59.90	724.0
60.90	3759.0
62.00	3468.0
62.90	2970.0
63.90	398.0
64.90	507.0
67.00	181.0
67.90	7496.0
68.90	7524.0
69.90	588.0
71.90	394.0
72.90	3386.0
74.00	12486.0
75.00	37680.0
75.90	3534.0
76.80	531.0
77.90	245.0
78.80	2113.0
79.90	707.0
80.90	2181.0
81.80	521.0
85.70	104.0
86.90	3262.0
87.90	3070.0
90.80	334.0
91.90	1985.0
92.90	3083.0
94.00	8245.0
94.90	74928.0
96.00	5089.0
97.00	182.0
103.90	285.0
105.80	291.0
115.80	296.0
116.80	538.0
117.80	252.0
118.90	360.0
127.70	206.0
128.80	134.0
129.80	241.0
134.80	136.0
140.80	577.0
142.80	638.0
145.70	116.0
147.80	123.0
154.80	211.0
156.80	133.0
171.90	628.0
172.90	485.0
173.90	57048.0
174.90	4299.0
175.90	55944.0
176.90	3571.0
177.80	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005