

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081022\
 Data File : VU050215.D
 Acq On : 10 Aug 2022 13:36
 Operator : SY/MD
 Sample : VU0810WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0810WBL01

Quant Time: Aug 10 16:27:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081022DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Aug 10 15:54:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	29186	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	8123	0.811	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	8548	0.845	ug/l	0.00
Spiked Amount 1.000			Recovery	=	84.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081022\
Data File : VU050215.D
Acq On : 10 Aug 2022 13:36
Operator : SY/MD
Sample : VU0810WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0810WBL01

Quant Time: Aug 10 16:27:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081022DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Aug 10 15:54:10 2022
Response via : Initial Calibration




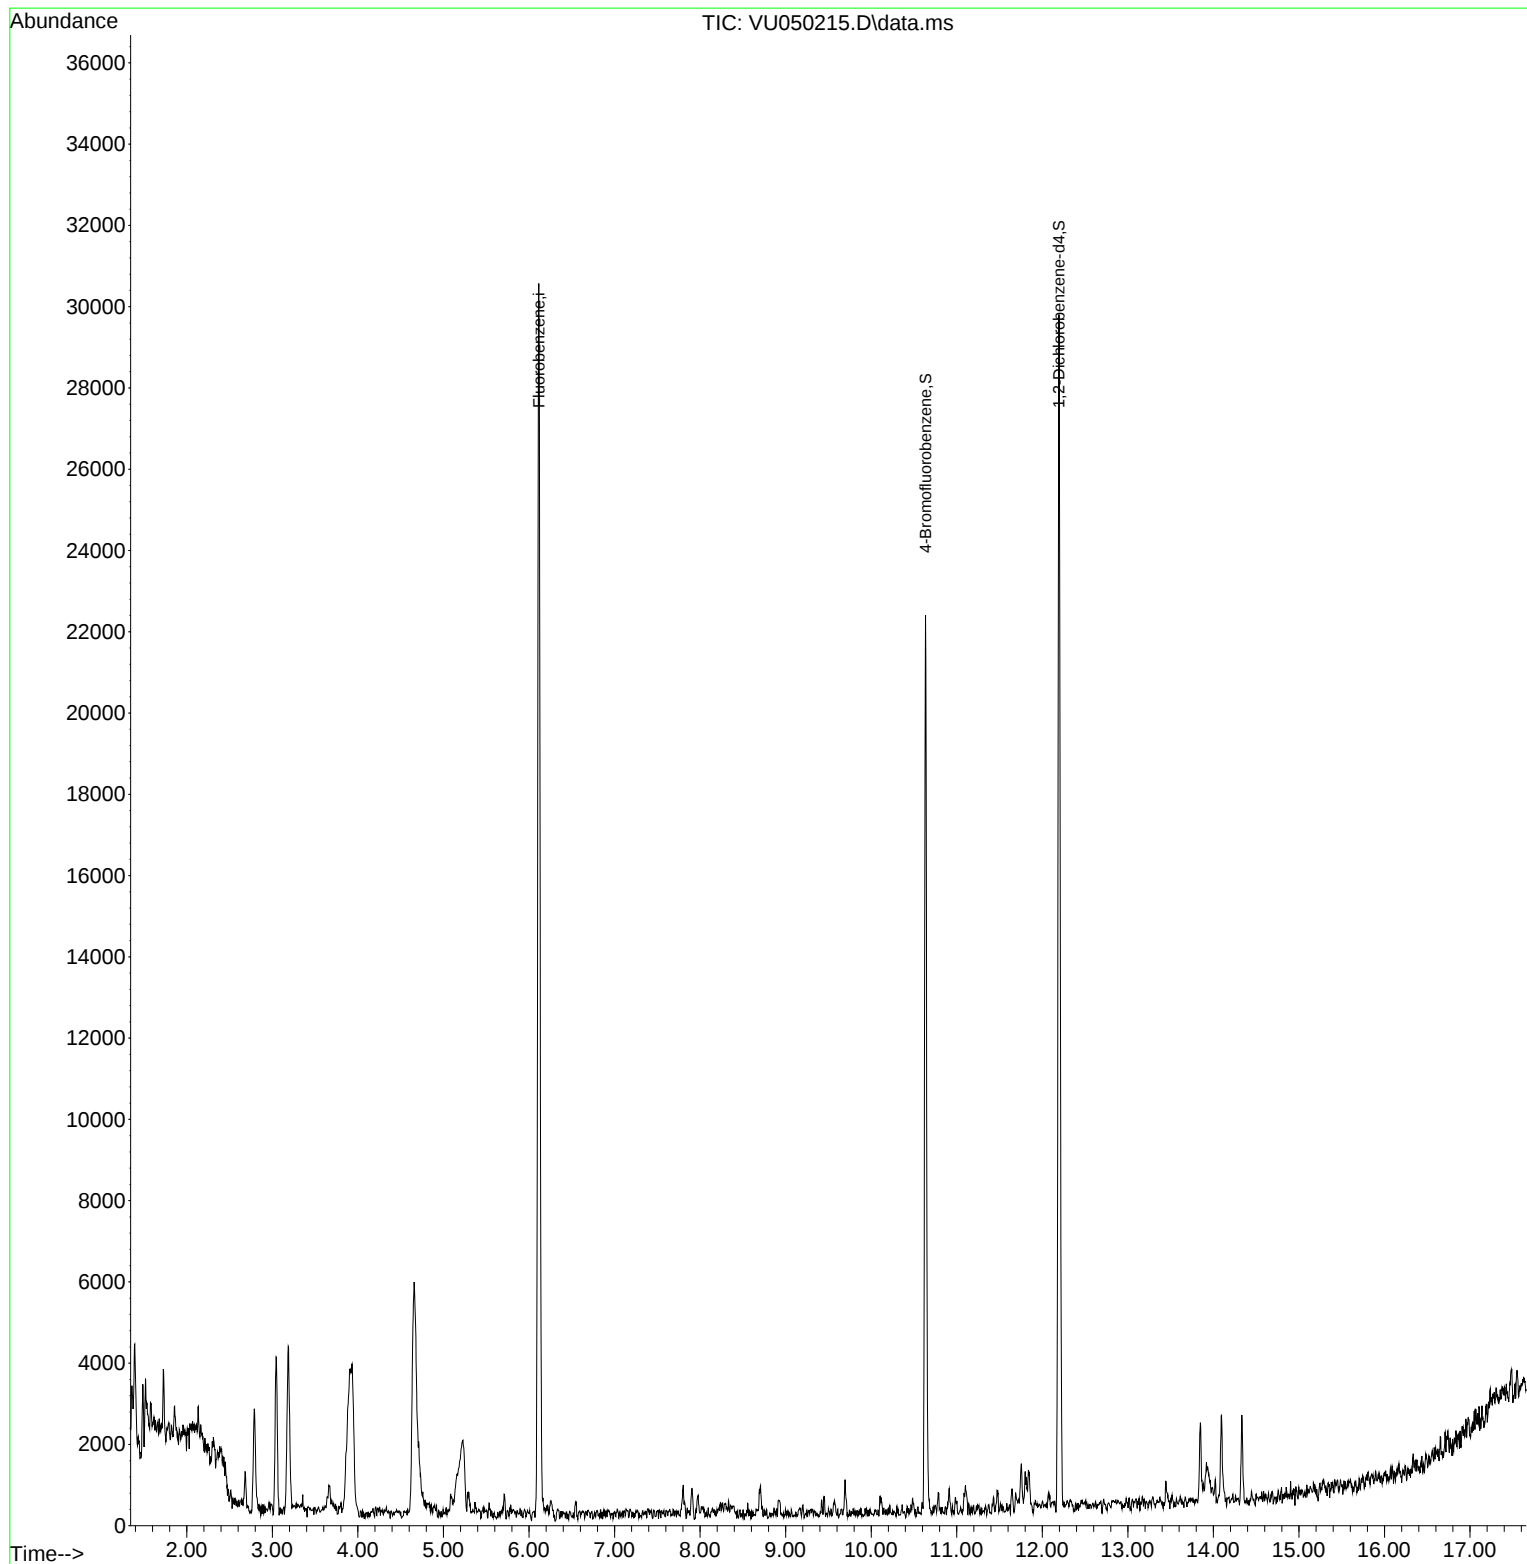


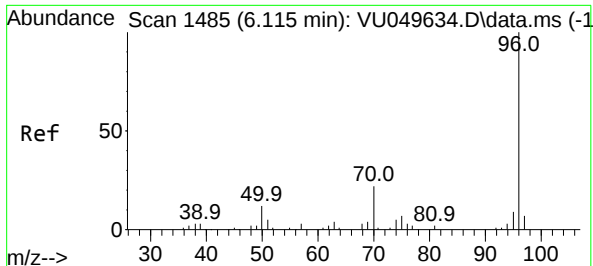

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU050215.D
Acq: 10 Aug 2022 13:36




Instrument :
MSVOA_U
ClientSampleId :
VU0810WBL01


Tgt Ion: 96	Resp: 29186
Ion Ratio	Lower Upper
96 100	
70 19.6	16.7 25.1
95 9.2	7.4 11.0
97 6.7	0.0 0.0

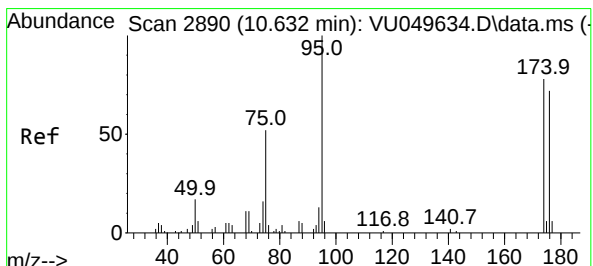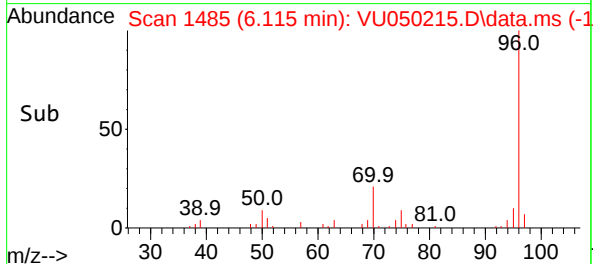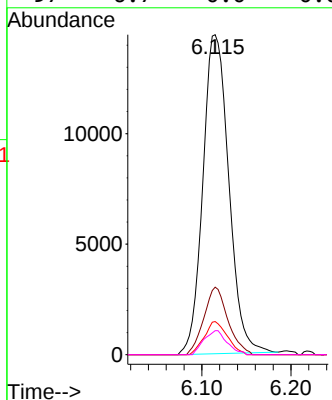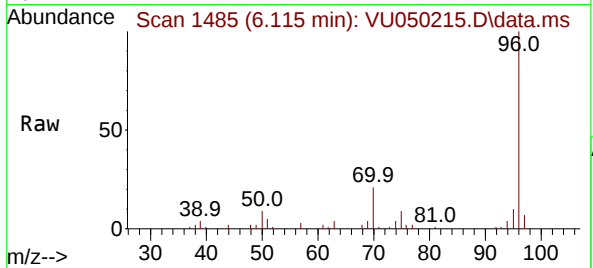

#57
4-Bromofluorobenzene
Concen: 0.811 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.004 min
Lab File: VU050215.D
Acq: 10 Aug 2022 13:36


Tgt Ion: 95	Resp: 8123
Ion Ratio	Lower Upper
95 100	
174 81.5	62.4 93.6
176 78.0	56.2 84.2

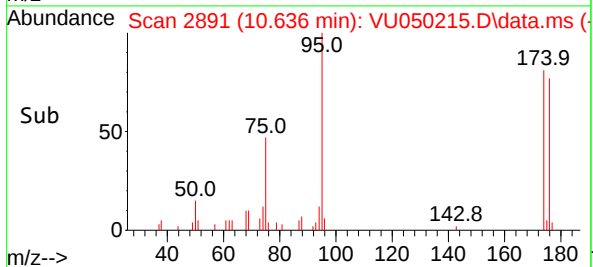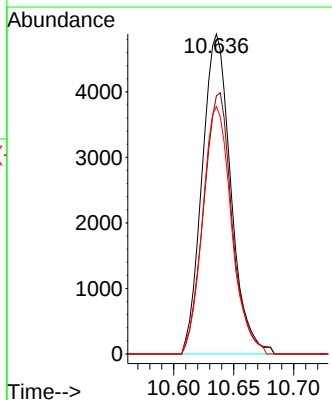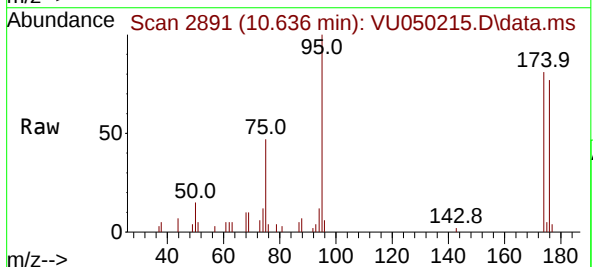

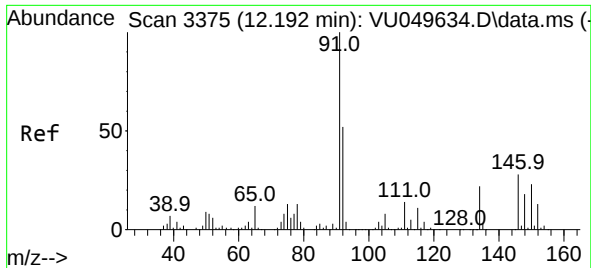

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.845 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU050215.D
 Acq: 10 Aug 2022 13:36

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0810WBL01

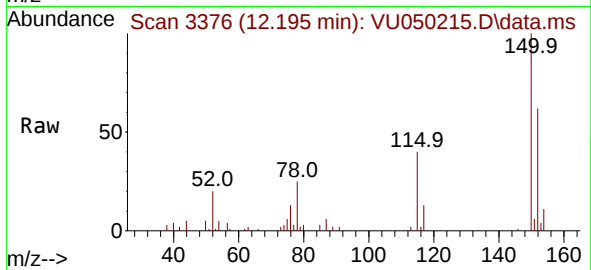

Tgt Ion:	152	Resp:	8548
Ion	Ratio	Lower	Upper
152	100		
115	64.8	0.0	254.6
150	162.1	0.0	623.6

