


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081022\
 Data File : VU050207.D
 Acq On : 10 Aug 2022 08:19
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081022DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Wed Aug 10 15:54:10 2022

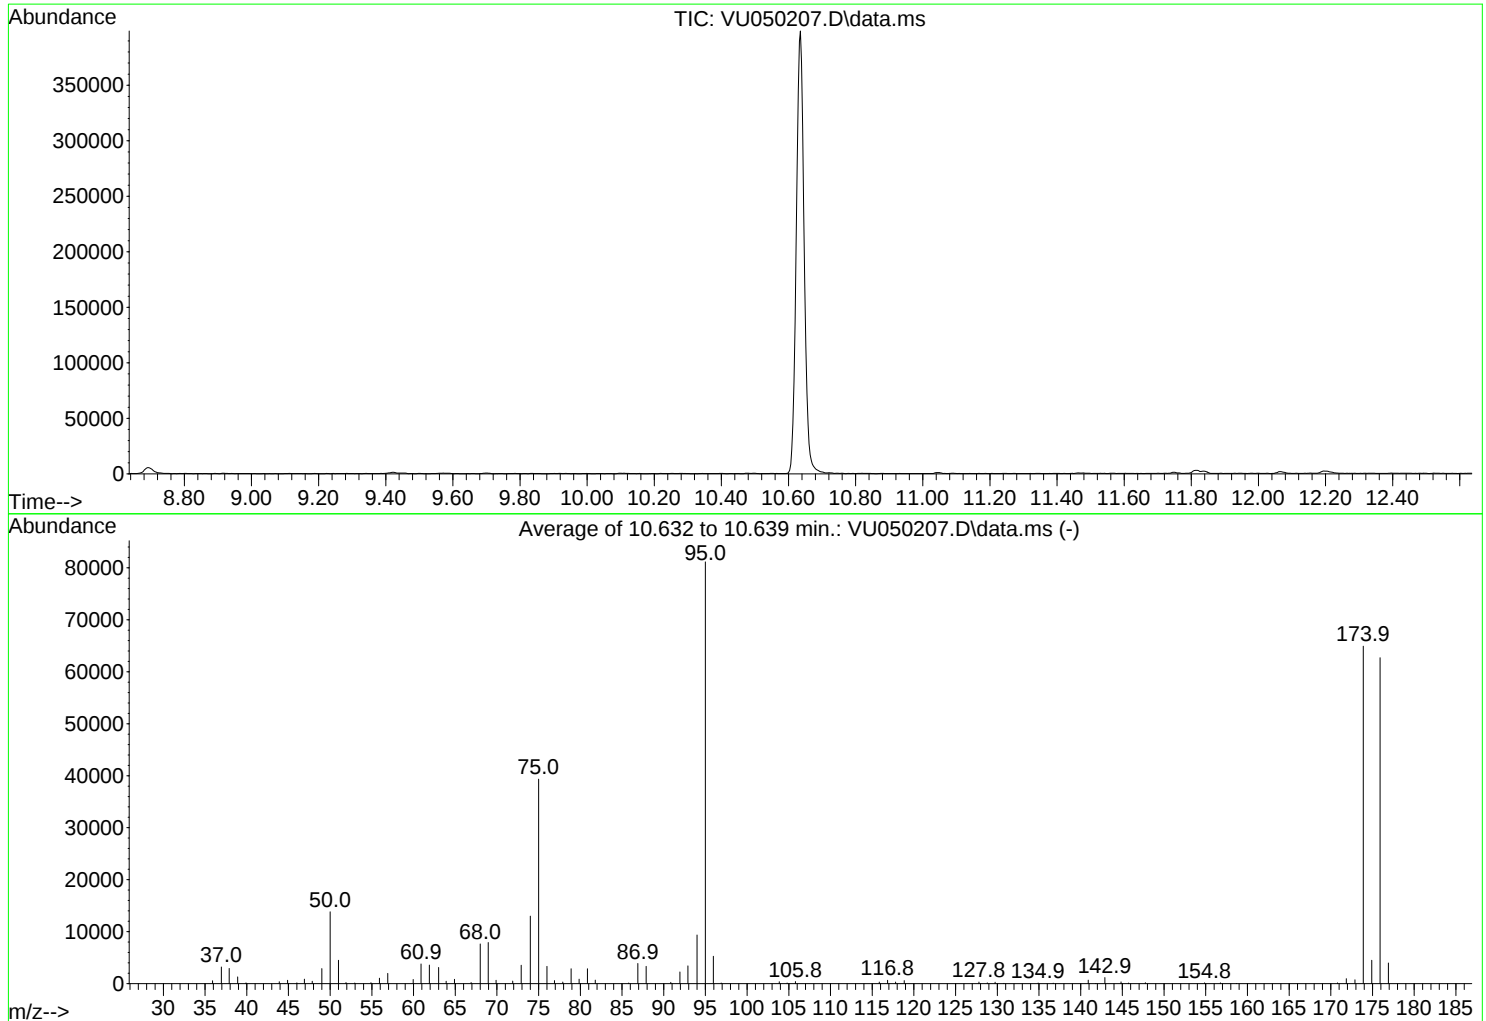

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	13826	PASS
75	95	30	60	48.5	39347	PASS
95	95	100	100	100.0	81147	PASS
96	95	5	9	6.5	5267	PASS
173	174	0.00	2	1.1	744	PASS
174	95	50	100	80.0	64928	PASS
175	174	5	9	6.9	4506	PASS
176	174	95	101	96.6	62712	PASS
177	176	5	9	6.3	3963	PASS