
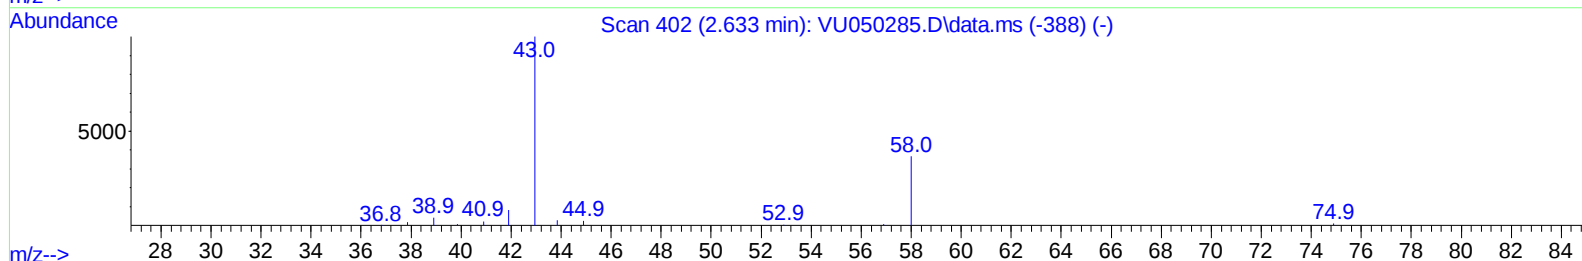
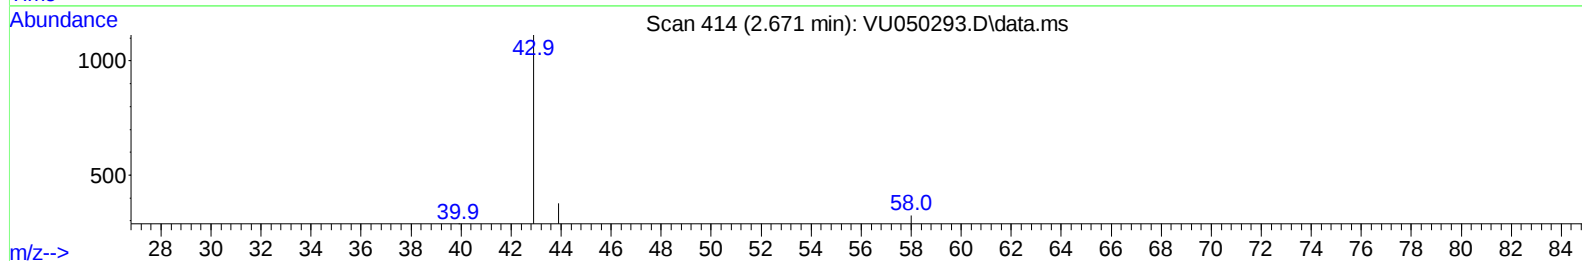


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050293.D
Acq On : 12 Aug 2022 20:28
Operator : SY/MD
Sample : N4072-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 13 01:23:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 01:20:27 2022
Response via : Initial Calibration

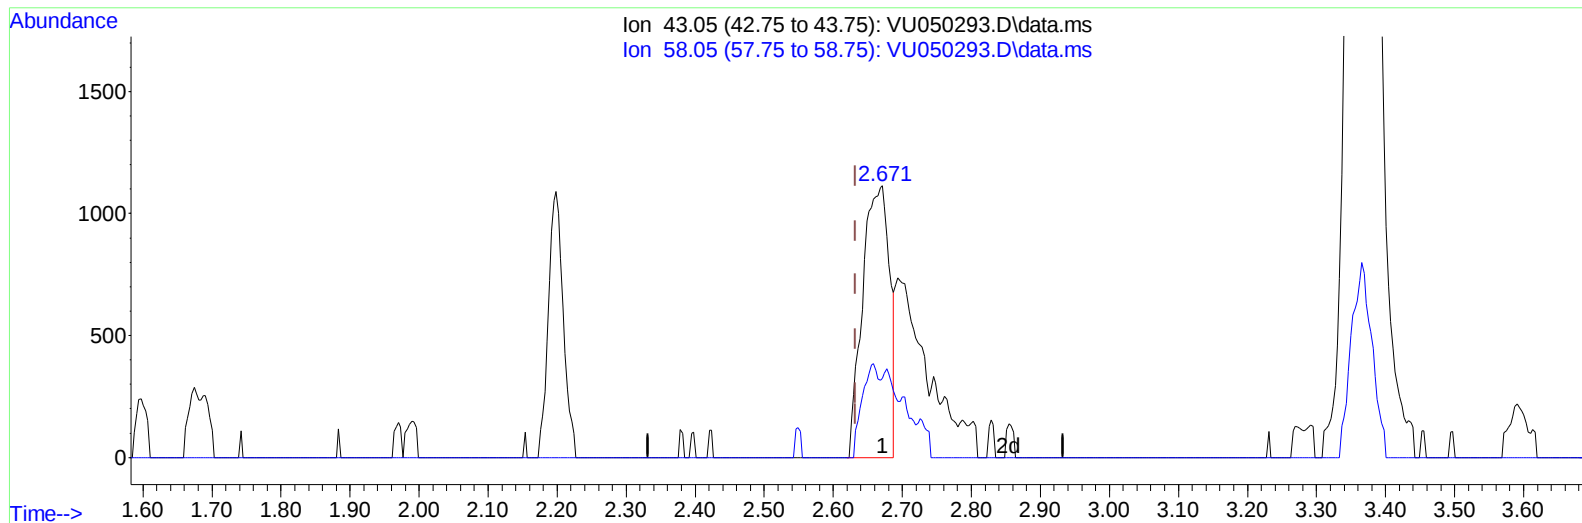

TIC: VU050293.D\data.ms

(13) Acetone (T)

2.671min (+ 0.038) 3.08 ug/L

response 3026

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.00	4.92
0.00	0.00	0.00
0.00	0.00	0.00