

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050246.D
 Acq On : 11 Aug 2022 22:54
 Operator : SY/MD
 Sample : N4160-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGBW5

Quant Time: Aug 12 05:01:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 04:56:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	91076	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	92758	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	34537	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	40950	5.403	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.000%
7) Chloroethane-d5	1.909	69	33143	5.420	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.400%
11) 1,1-Dichloroethene-d2	2.565	65	14565	4.917	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.400%
20) 2-Butanone-d5	4.629	46	98035	53.040	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.080%
24) Chloroform-d	5.063	84	70698	5.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.703	65	36986	5.110	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%
32) Benzene-d6	5.729	84	135612	4.685	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.694	67	47244	4.956	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.899	98	107238	4.195	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
43) trans-1,3-Dichloroprop...	8.182	79	14570	4.265	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.400%
46) 2-Hexanone-d5	8.636	63	54877	45.304	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.600%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	40265	4.810	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	34533	5.103	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						Qvalue
3) Chloromethane	1.520	50	1466	0.134	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050246.D
Acq On : 11 Aug 2022 22:54
Operator : SY/MD
Sample : N4160-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBW5

Quant Time: Aug 12 05:01:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 04:56:24 2022
Response via : Initial Calibration

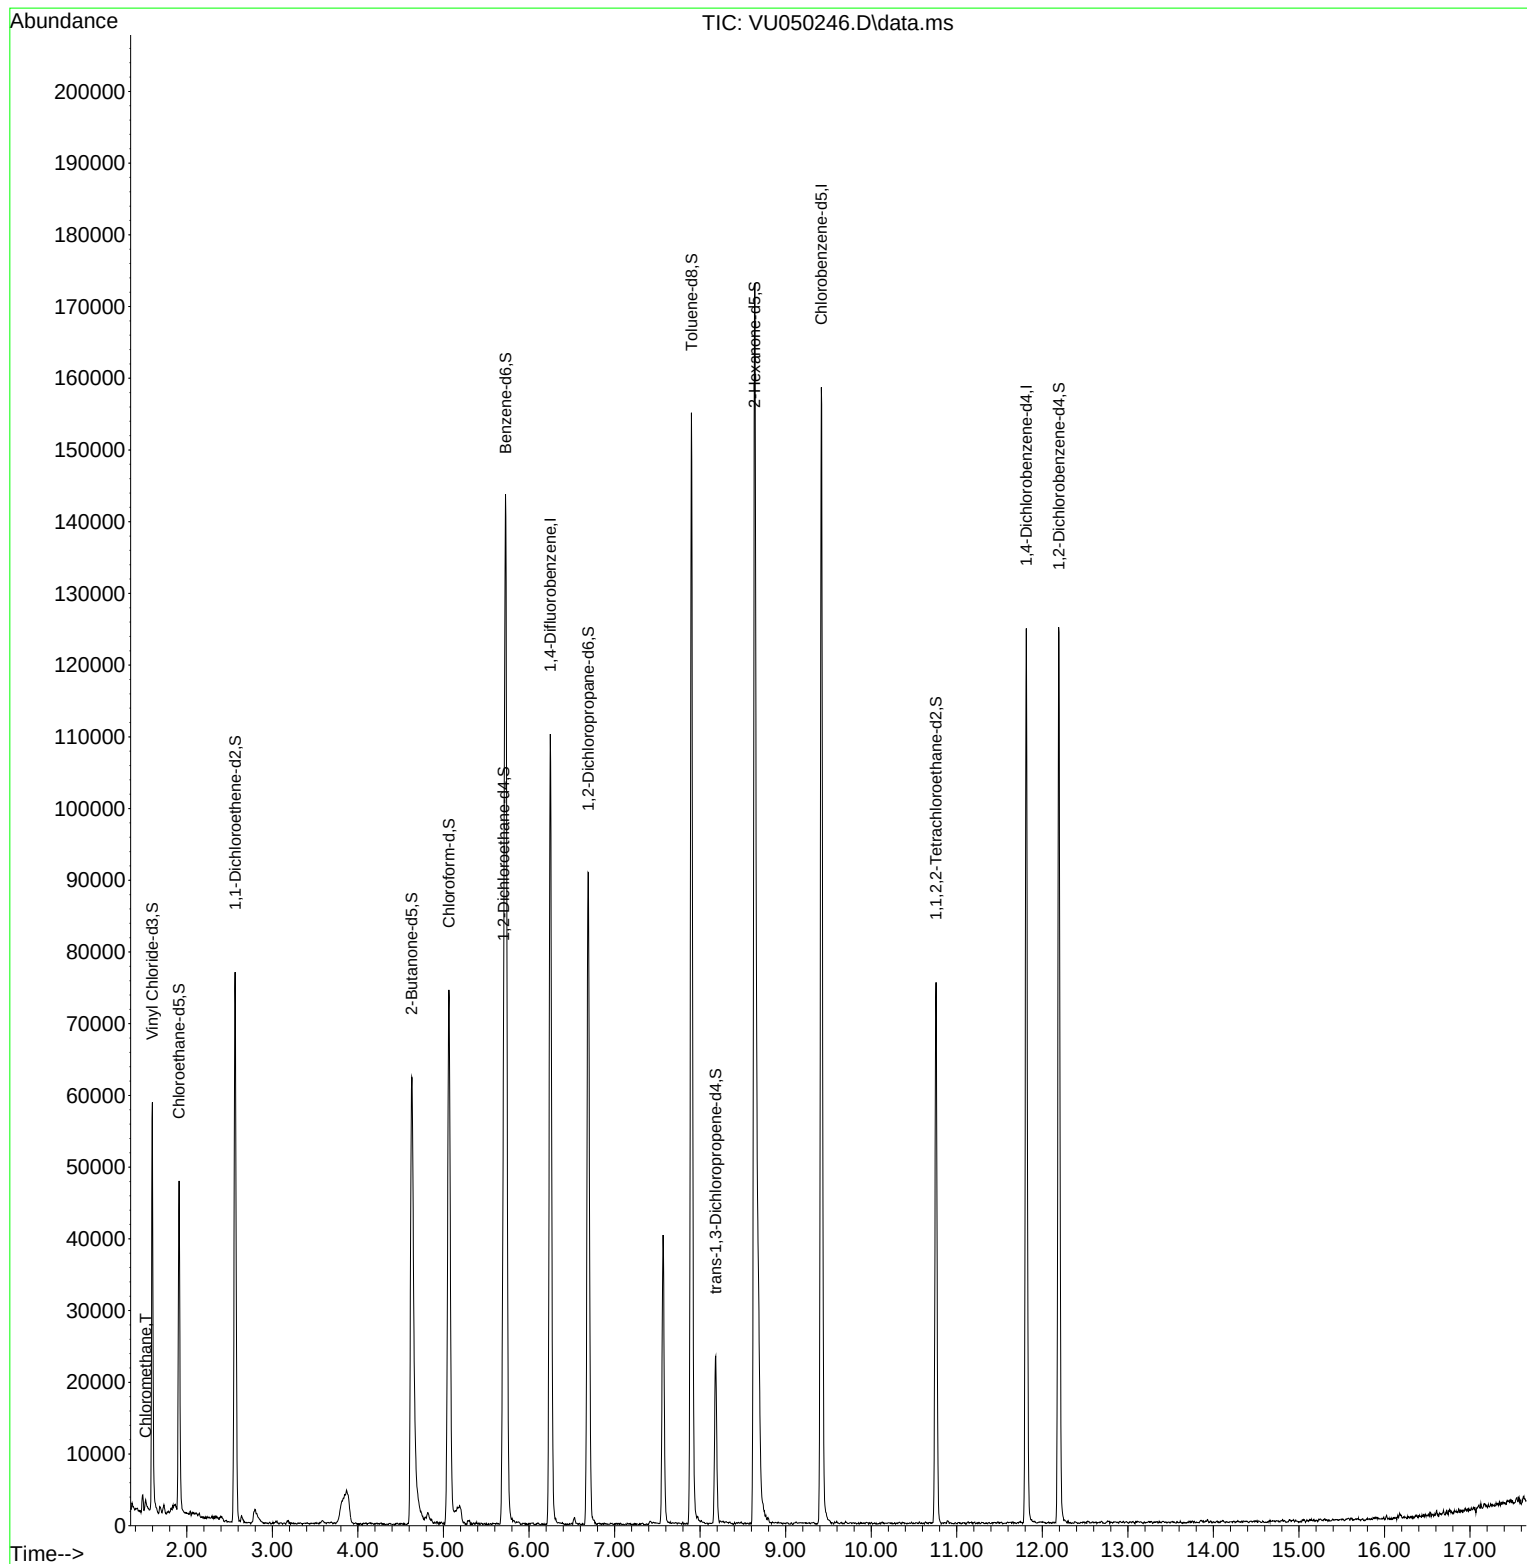

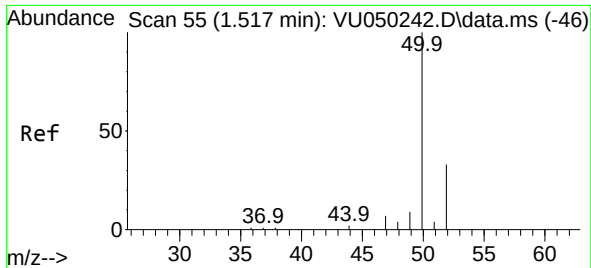

#3
 Chloromethane
 Concen: 0.134 ug/L
 RT: 1.520 min Scan# 50
 Delta R.T. 0.003 min
 Lab File: VU050246.D
 Acq: 11 Aug 2022 22:54

Instrument :
 MSVOA_U
 ClientSampleId :
 BGBW5

Tgt Ion: 50 Resp: 1466
 Ion Ratio Lower Upper
 50 100
 52 39.0 23.2 43.2

