

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050268.D
 Acq On : 12 Aug 2022 09:33
 Operator : SY/MD
 Sample : N4096-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJM6

Quant Time: Aug 12 23:12:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 23:11:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	101211	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	107353	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	39371	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	32410	3.848	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.000%
7) Chloroethane-d5	1.912	69	30724	4.521	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.400%
11) 1,1-Dichloroethene-d2	2.565	65	12572	3.819	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	4.629	46	100012	48.692	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.380%
24) Chloroform-d	5.063	84	67753	4.325	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.703	65	36595	4.549	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	5.729	84	123068	3.674	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.400%
36) 1,2-Dichloropropane-d6	6.690	67	43928	3.982	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.600%
41) Toluene-d8	7.899	98	91669	3.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	62.000%#
43) trans-1,3-Dichloroprop...	8.179	79	12620	3.192	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.800%
46) 2-Hexanone-d5	8.636	63	42157	30.071	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	60.140%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	40099	4.139	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	32223	4.177	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.600%
Target Compounds						Qvalue
13) Acetone	2.639	43	9389	8.208	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050268.D
Acq On : 12 Aug 2022 09:33
Operator : SY/MD
Sample : N4096-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJM6

Quant Time: Aug 12 23:12:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 23:11:34 2022
Response via : Initial Calibration

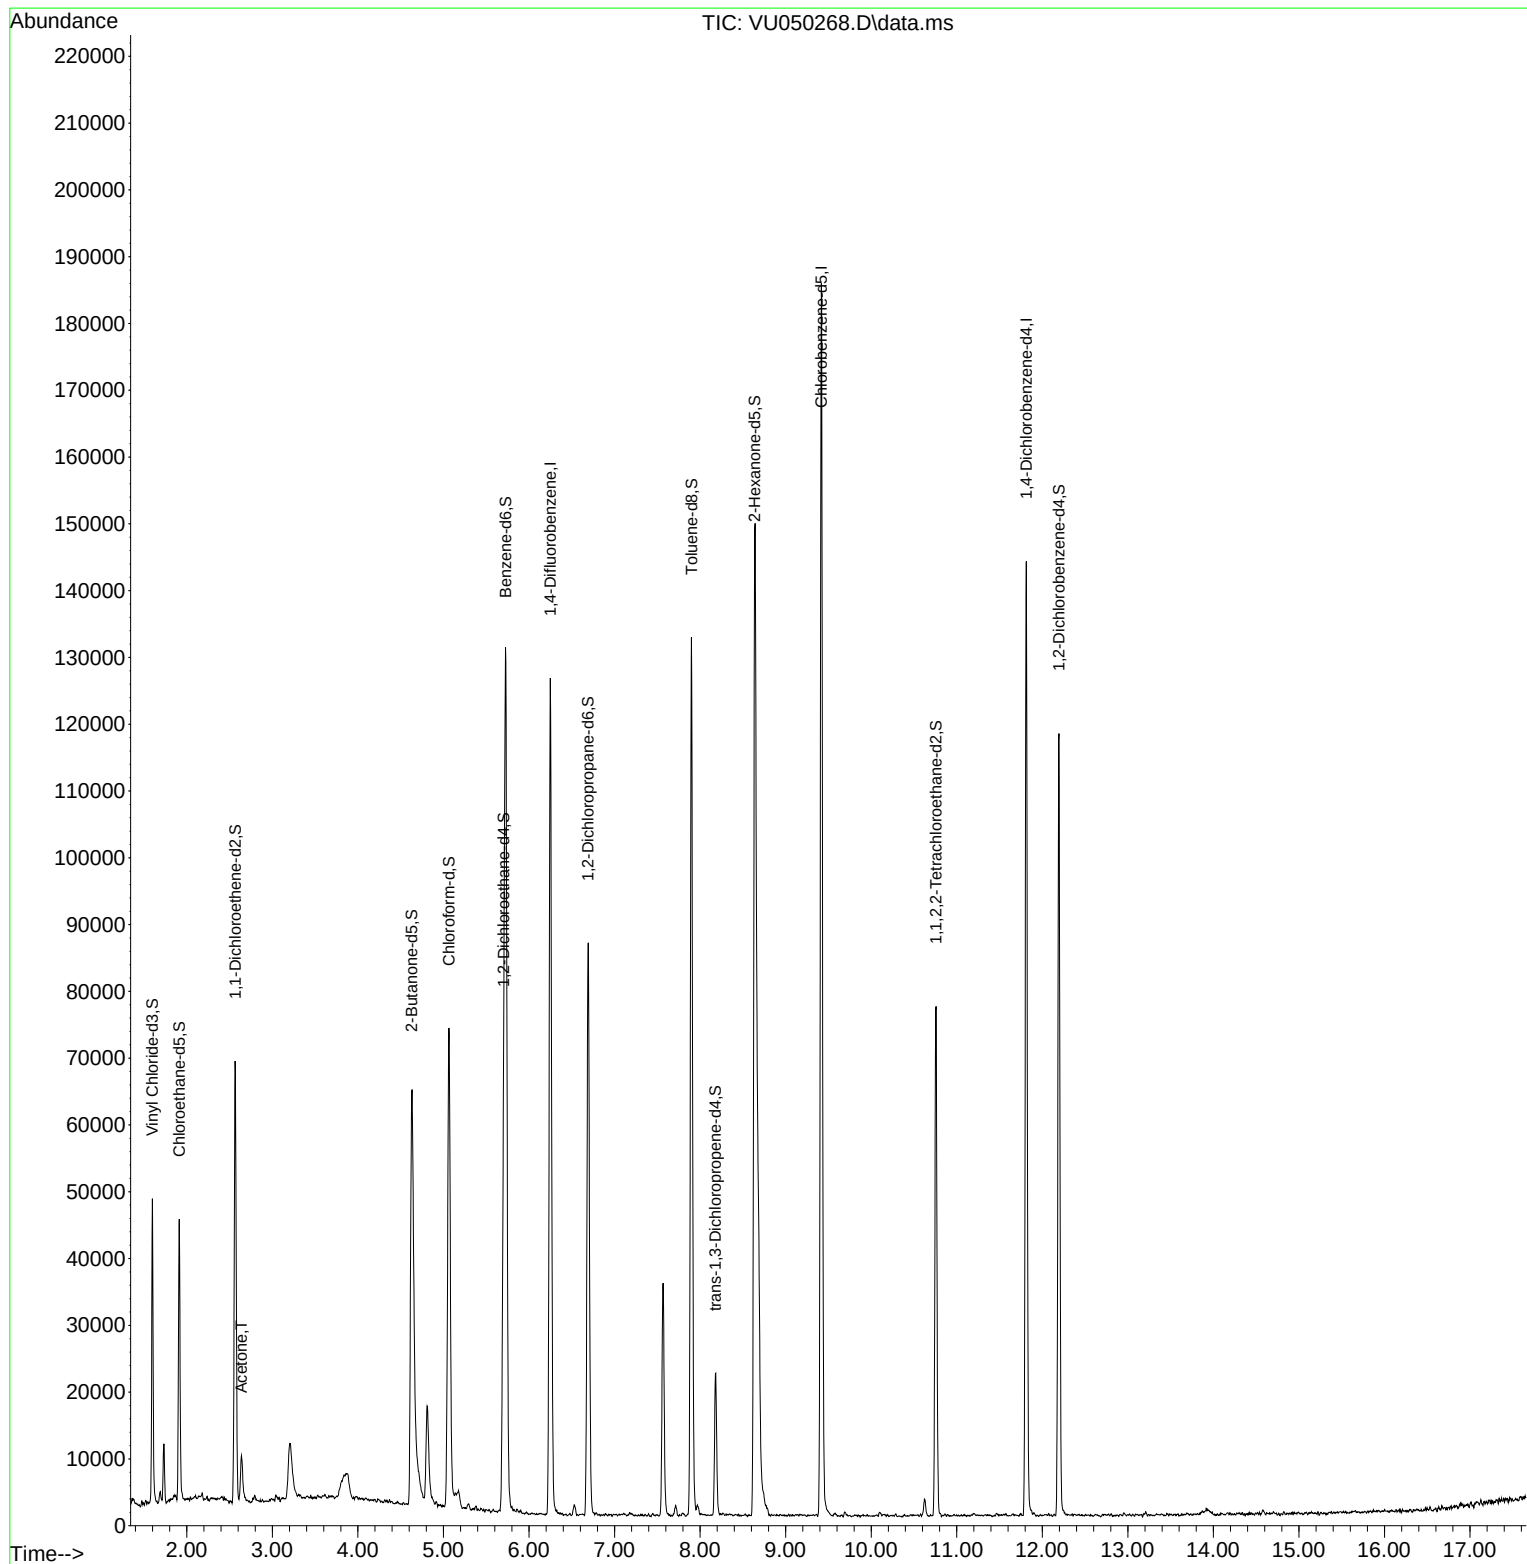

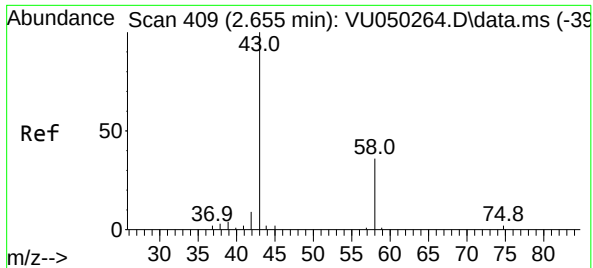

#13
 Acetone
 Concen: 8.208 ug/L
 RT: 2.639 min Scan# 40
 Delta R.T. -0.016 min
 Lab File: VU050268.D
 Acq: 12 Aug 2022 09:33

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJM6

Tgt Ion: 43 Resp: 9389
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 64.0

