

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050269.D
 Acq On : 12 Aug 2022 09:57
 Operator : SY/MD
 Sample : N4096-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJM7

Quant Time: Aug 12 23:13:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 23:11:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	100281	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	104203	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	39419	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	33913	4.064	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.912	69	31682	4.705	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.200%
11) 1,1-Dichloroethene-d2	2.565	65	12809	3.927	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.600%
20) 2-Butanone-d5	4.629	46	101255	49.754	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.500%
24) Chloroform-d	5.063	84	70857	4.565	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.703	65	37591	4.717	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.729	84	131104	4.032	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.600%
36) 1,2-Dichloropropane-d6	6.690	67	45933	4.289	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.800%
41) Toluene-d8	7.899	98	99110	3.451	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.000%#
43) trans-1,3-Dichloroprop...	8.179	79	13430	3.500	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.636	63	44560	32.746	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	65.500%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	41793	4.444	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	34498	4.467	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.400%
Target Compounds					Qvalue	
13) Acetone	2.636	43	6646	5.864	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050269.D
Acq On : 12 Aug 2022 09:57
Operator : SY/MD
Sample : N4096-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJM7


Quant Time: Aug 12 23:13:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 23:11:34 2022
Response via : Initial Calibration

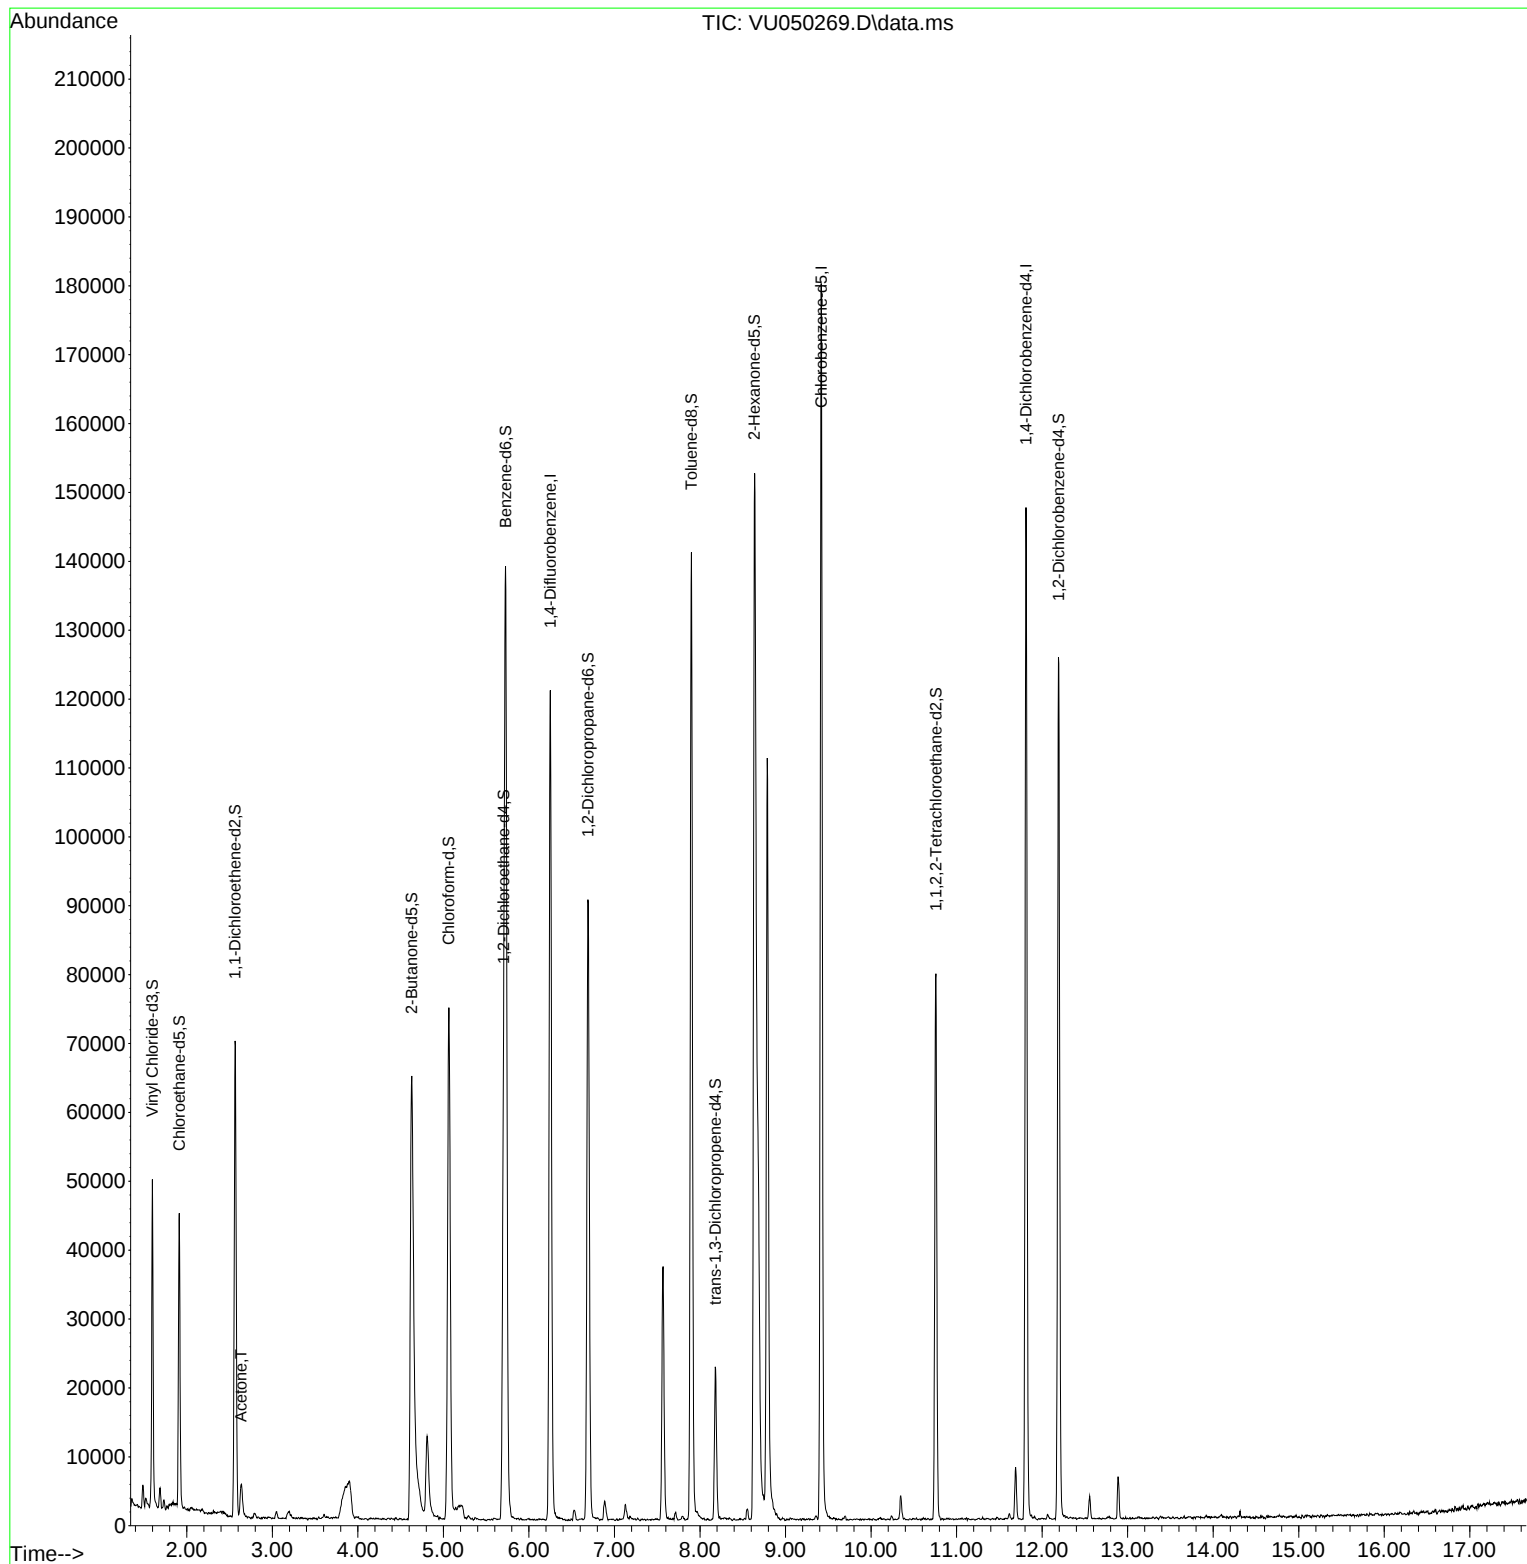

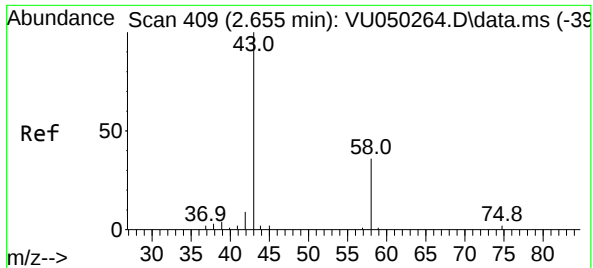

#13
 Acetone
 Concen: 5.864 ug/L
 RT: 2.636 min Scan# 40
 Delta R.T. -0.019 min
 Lab File: VU050269.D
 Acq: 12 Aug 2022 09:57

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJM7

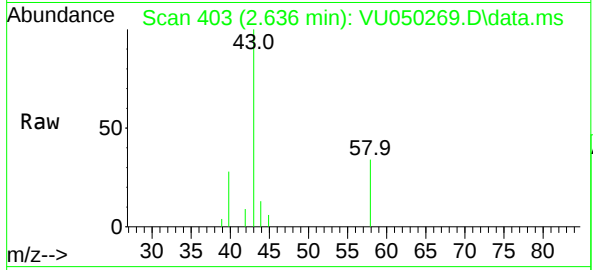

Tgt Ion:	43	Resp:	6646
Ion Ratio	Lower	Upper	
43	100		
58	34.4	0.0	64.0

