

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050282.D
 Acq On : 12 Aug 2022 15:17
 Operator : SY/MD
 Sample : N4072-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUT7

Quant Time: Aug 12 23:17:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 12 23:11:34 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	83719	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	84637	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	32962	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	34916	5.012	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.200%		
7) Chloroethane-d5	1.909	69	29998	5.337	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 106.800%		
11) 1,1-Dichloroethene-d2	2.565	65	12919	4.744	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 94.800%		
20) 2-Butanone-d5	4.626	46	94360	55.538	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	= 111.080%		
24) Chloroform-d	5.063	84	65619	5.064	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 101.200%		
26) 1,2-Dichloroethane-d4	5.703	65	35827	5.384	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 107.600%		
32) Benzene-d6	5.729	84	123865	4.690	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 93.800%		
36) 1,2-Dichloropropane-d6	6.694	67	43455	4.996	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 100.000%		
41) Toluene-d8	7.899	98	94944	4.070	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 81.400%		
43) trans-1,3-Dichloroprop...	8.182	79	13964	4.480	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 89.600%		
46) 2-Hexanone-d5	8.636	63	47030	42.551	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 85.100%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37527	4.913	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 98.200%		
66) 1,2-Dichlorobenzene-d4	12.195	152	32093	4.969	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 99.400%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.517	50	1587	0.158	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050282.D
Acq On : 12 Aug 2022 15:17
Operator : SY/MD
Sample : N4072-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUT7


Quant Time: Aug 12 23:17:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 12 23:11:34 2022
Response via : Initial Calibration

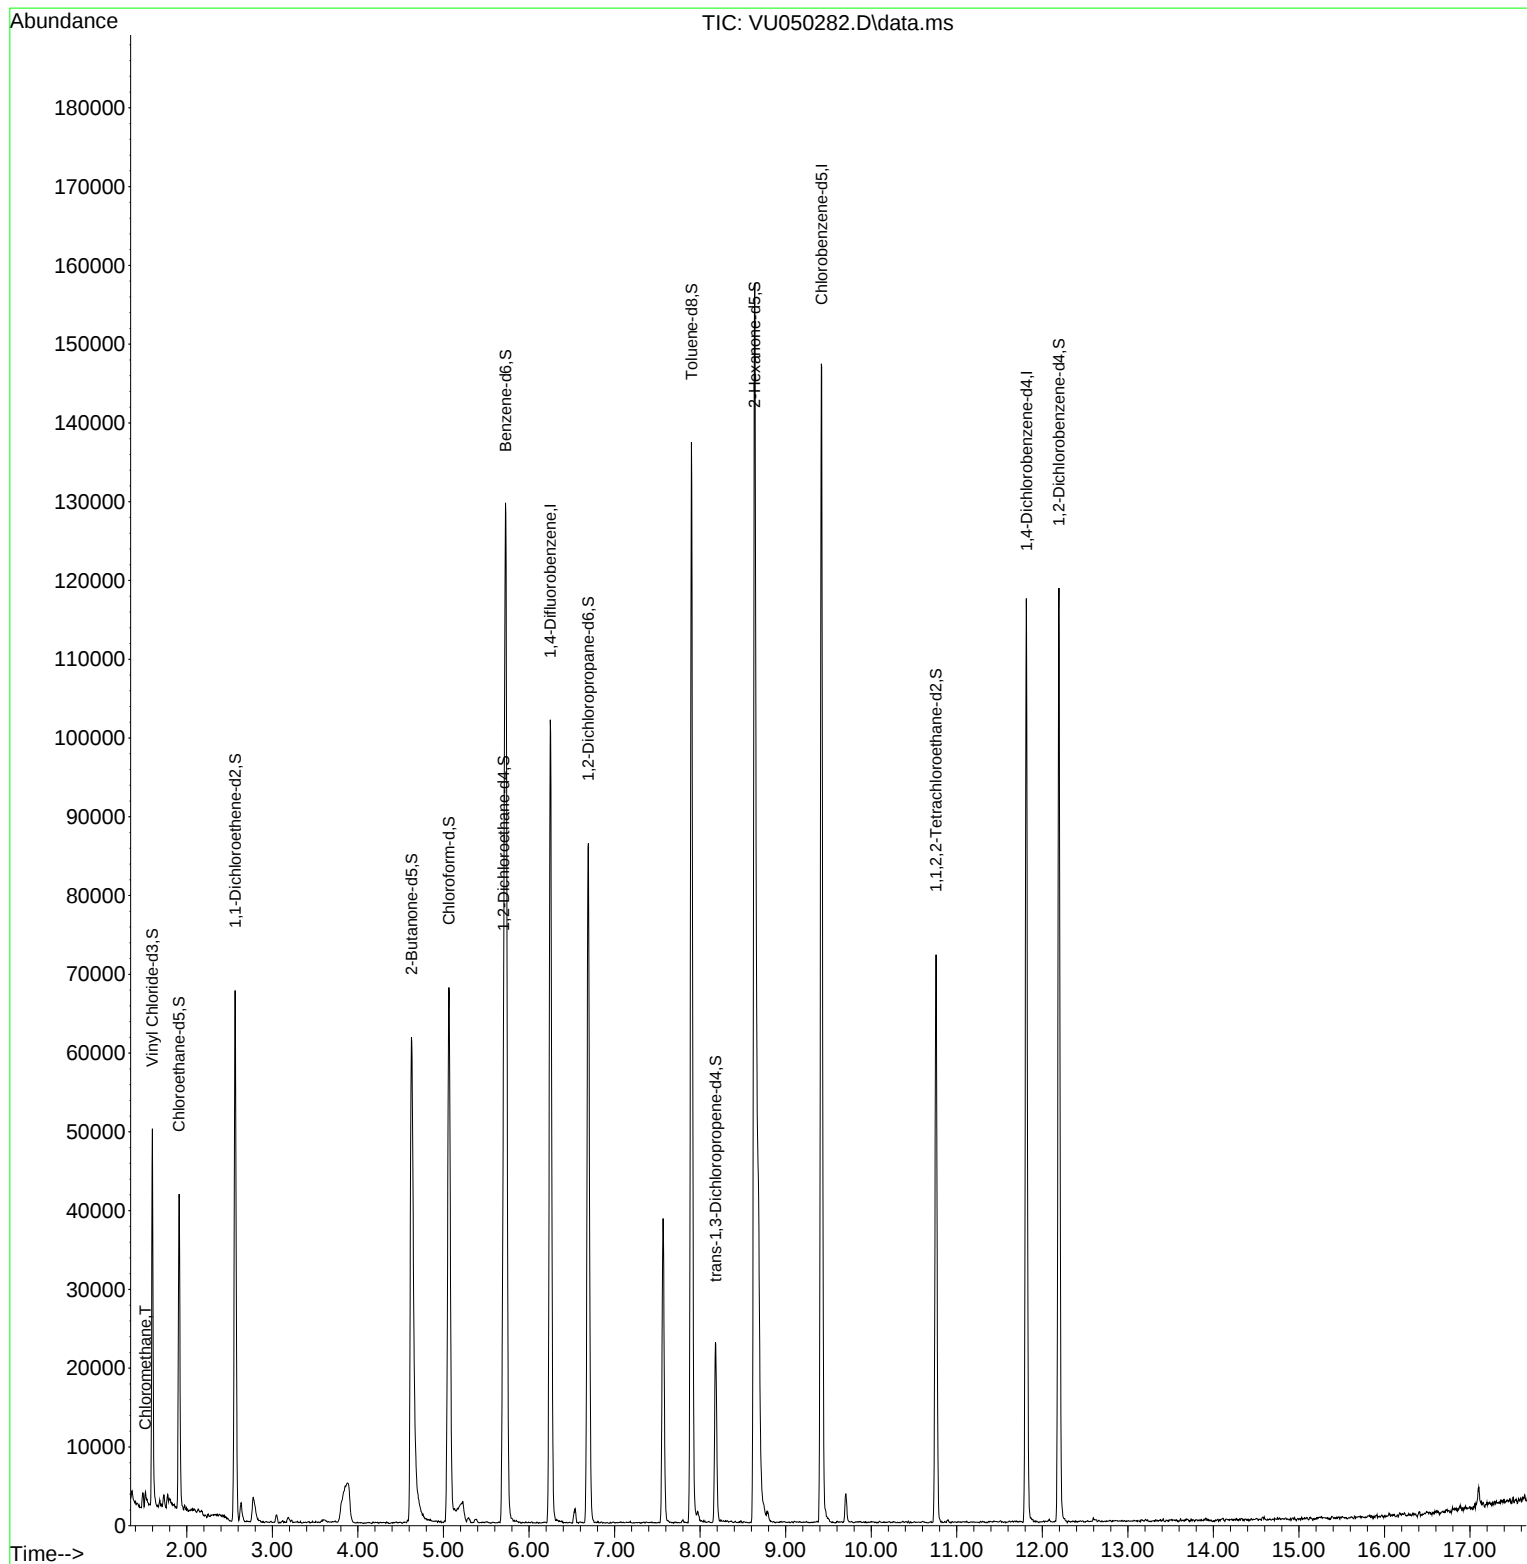

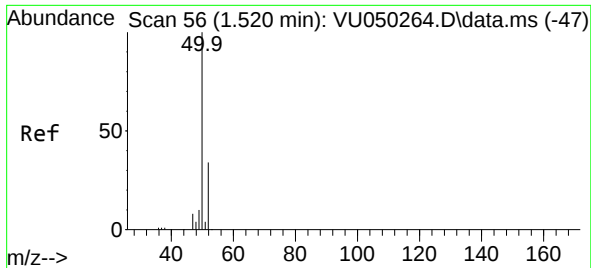

#3
 Chloromethane
 Concen: 0.158 ug/L
 RT: 1.517 min Scan# 51
 Delta R.T. -0.003 min
 Lab File: VU050282.D
 Acq: 12 Aug 2022 15:17

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUT7

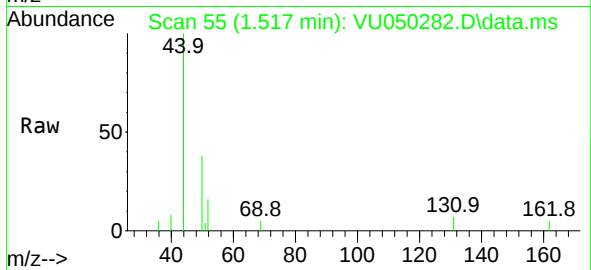

Tgt Ion: 50 Resp: 1587
 Ion Ratio Lower Upper
 50 100
 52 41.8 23.2 43.2

