

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050289.D
 Acq On : 12 Aug 2022 18:50
 Operator : SY/MD
 Sample : N4072-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUU4

Quant Time: Aug 13 01:22:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 01:20:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	86128	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	86771	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	34243	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	33157	4.626	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%
7) Chloroethane-d5	1.909	69	28304	4.895	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	2.565	65	11802	4.213	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.200%
20) 2-Butanone-d5	4.626	46	92195	52.746	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.500%
24) Chloroform-d	5.064	84	62142	4.661	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.704	65	33662	4.918	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.729	84	115663	4.271	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
36) 1,2-Dichloropropane-d6	6.691	67	40649	4.559	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.200%
41) Toluene-d8	7.900	98	87602	3.663	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%
43) trans-1,3-Dichloroprop...	8.183	79	13193	4.129	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.600%
46) 2-Hexanone-d5	8.636	63	50664	44.712	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.420%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	36560	4.669	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	31030	4.625	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.400%
Target Compounds						Qvalue
13) Acetone	2.633	43	4516	4.639	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050289.D
Acq On : 12 Aug 2022 18:50
Operator : SY/MD
Sample : N4072-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUU4

Quant Time: Aug 13 01:22:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 01:20:27 2022
Response via : Initial Calibration

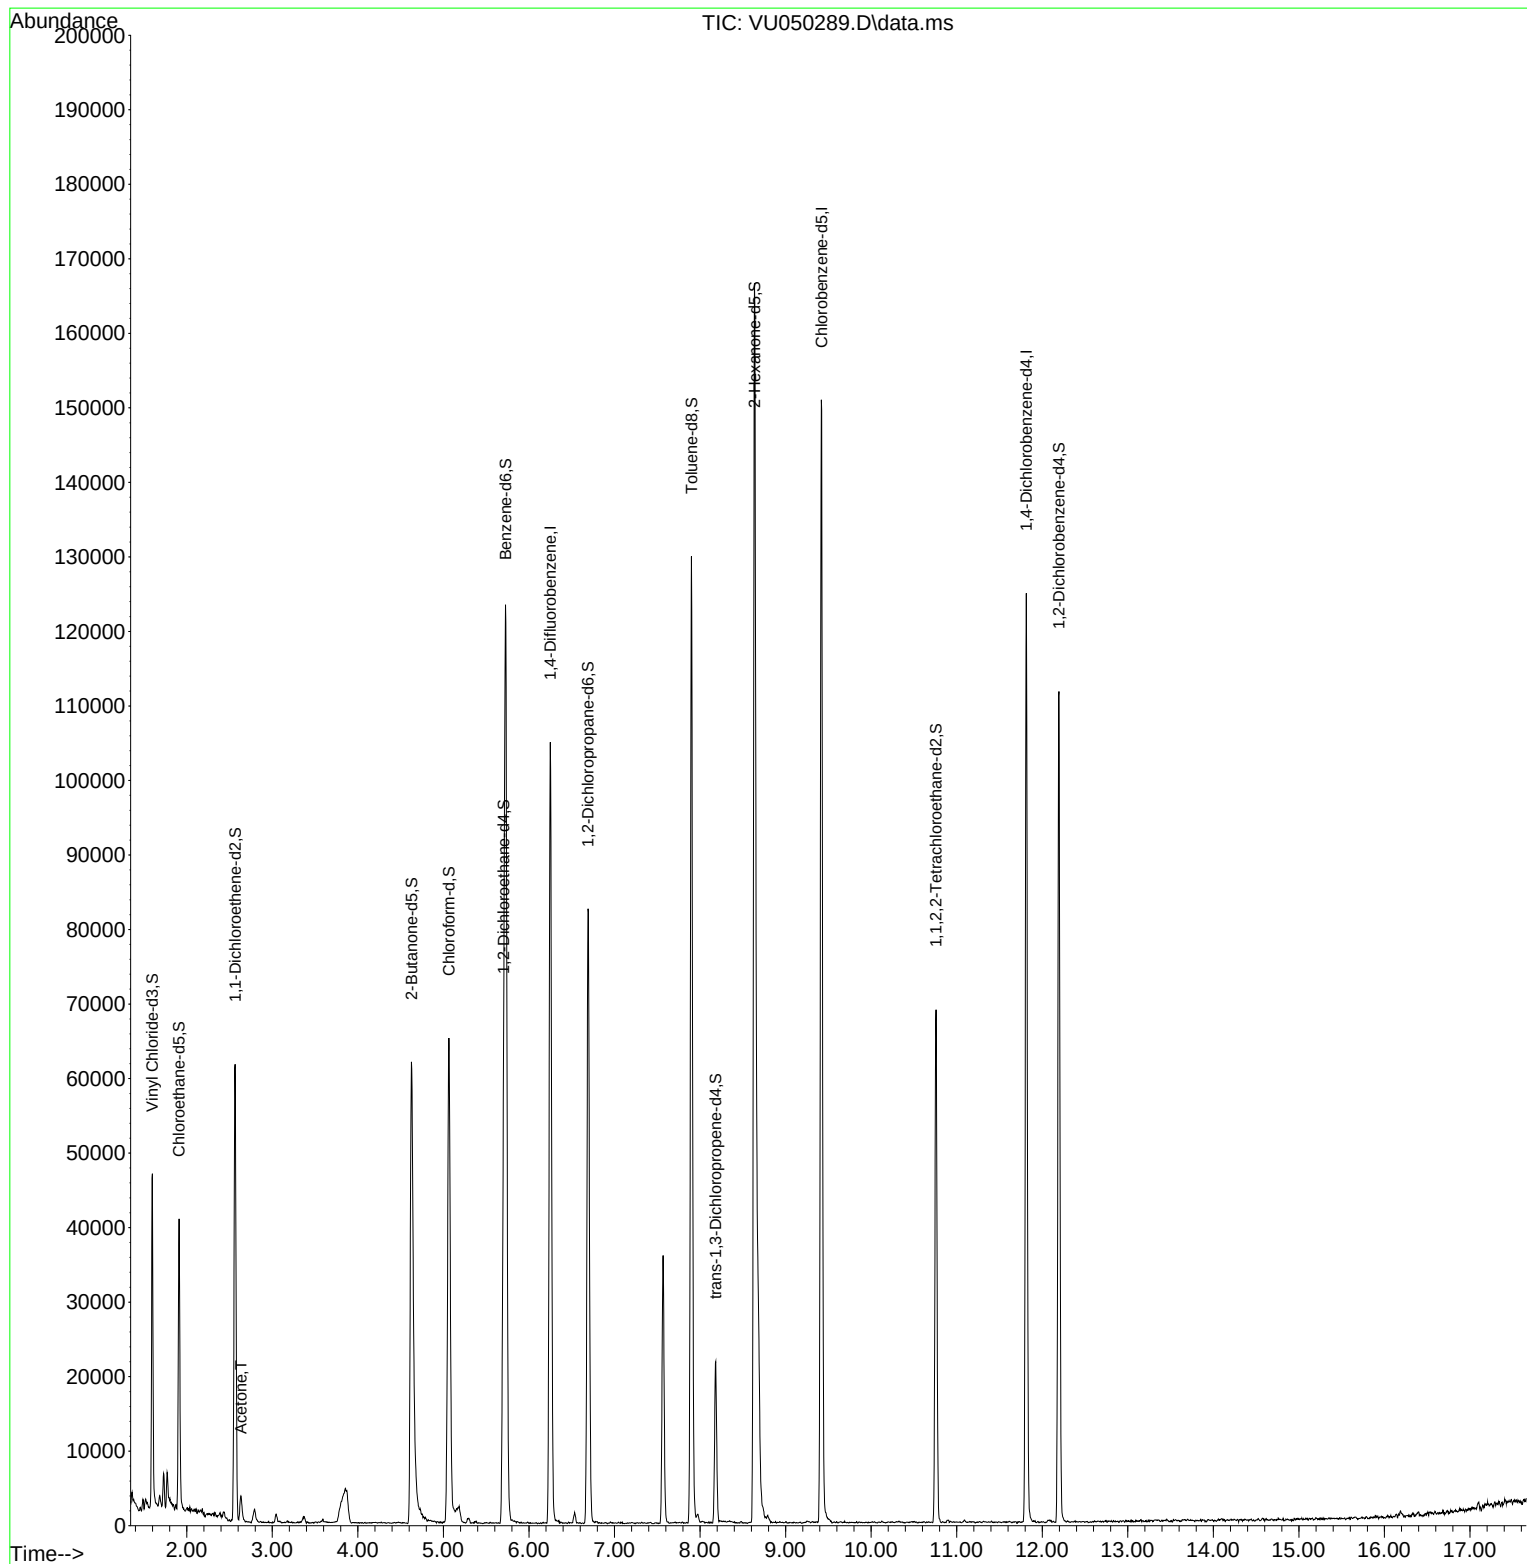

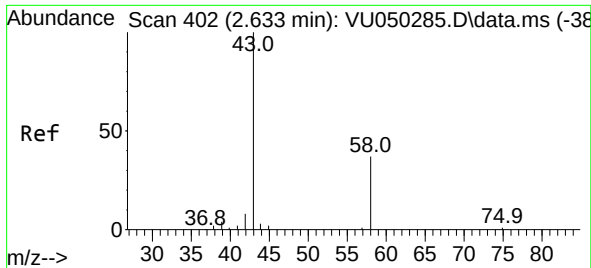

#13

Acetone

Concen: 4.639 ug/L

RT: 2.633 min Scan# 40

Delta R.T. 0.000 min

Lab File: VU050289.D


Acq: 12 Aug 2022 18:50

Instrument :

MSVOA_U

ClientSampleId :

DBUU4

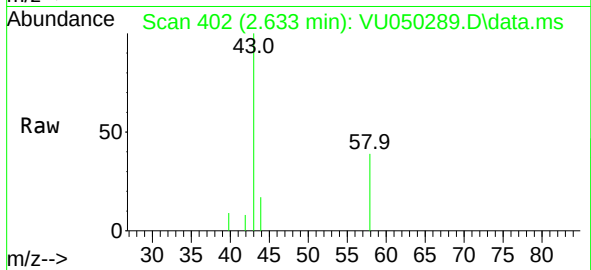

Tgt Ion: 43 Resp: 4516

Ion Ratio Lower Upper

43 100

58 34.6 0.0 64.0

