

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050236.D
 Acq On : 11 Aug 2022 17:33
 Operator : SY/MD
 Sample : N4160-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGBT6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	38	44	51	rBV2	4489	5024	1.22%	0.168%
2	1.597	72	80	99	rVV	57456	65237	15.83%	2.175%
3	1.909	169	177	189	rBV	47528	60320	14.63%	2.011%
4	2.565	369	381	394	rBV	82048	130984	31.78%	4.367%
5	2.787	437	450	462	rBV3	4195	9292	2.25%	0.310%
6	3.819	748	771	773	rBV	3114	8085	1.96%	0.270%
7	4.629	1008	1023	1061	rBV	63193	175202	42.50%	5.842%
8	5.063	1141	1158	1174	rBV	74300	163900	39.76%	5.465%
9	5.726	1343	1364	1389	rBV2	145287	378851	91.91%	12.632%
10	6.250	1513	1527	1548	rBV	101550	193542	46.95%	6.453%
11	6.546	1606	1619	1637	rBV2	35000	67382	16.35%	2.247%
12	6.694	1652	1665	1682	rBV	92669	178487	43.30%	5.951%
13	7.568	1924	1937	1954	rBV	42112	73407	17.81%	2.448%
14	7.899	2026	2040	2057	rBV	158422	277668	67.36%	9.258%
15	7.973	2057	2063	2072	rVB3	3528	5719	1.39%	0.191%
16	8.182	2118	2128	2145	rBV	25712	43039	10.44%	1.435%
17	8.636	2257	2269	2308	rBV3	174678	412220	100.00%	13.745%
18	9.417	2500	2512	2532	rBV	144882	240664	58.38%	8.025%
19	10.758	2918	2929	2953	rVB	75352	120525	29.24%	4.019%
20	11.812	3246	3257	3274	rBV	111690	181689	44.08%	6.058%
21	12.195	3362	3376	3400	rBV	129577	207872	50.43%	6.931%




Sum of corrected areas: 2999109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050236.D
Acq On : 11 Aug 2022 17:33
Operator : SY/MD
Sample : N4160-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

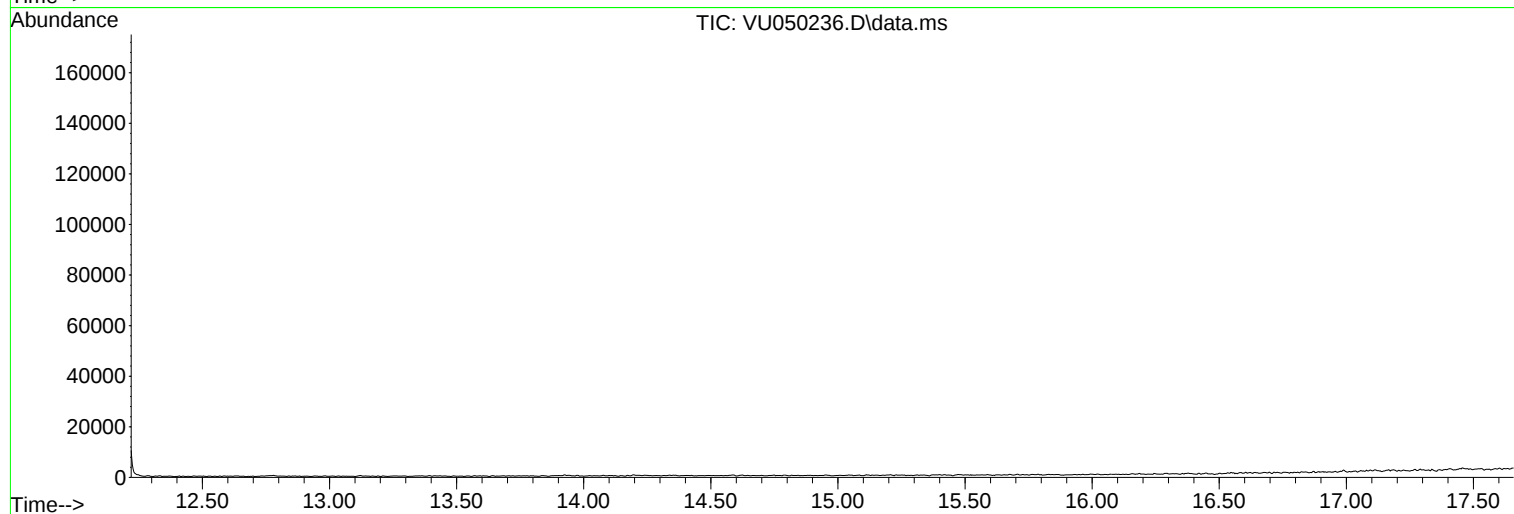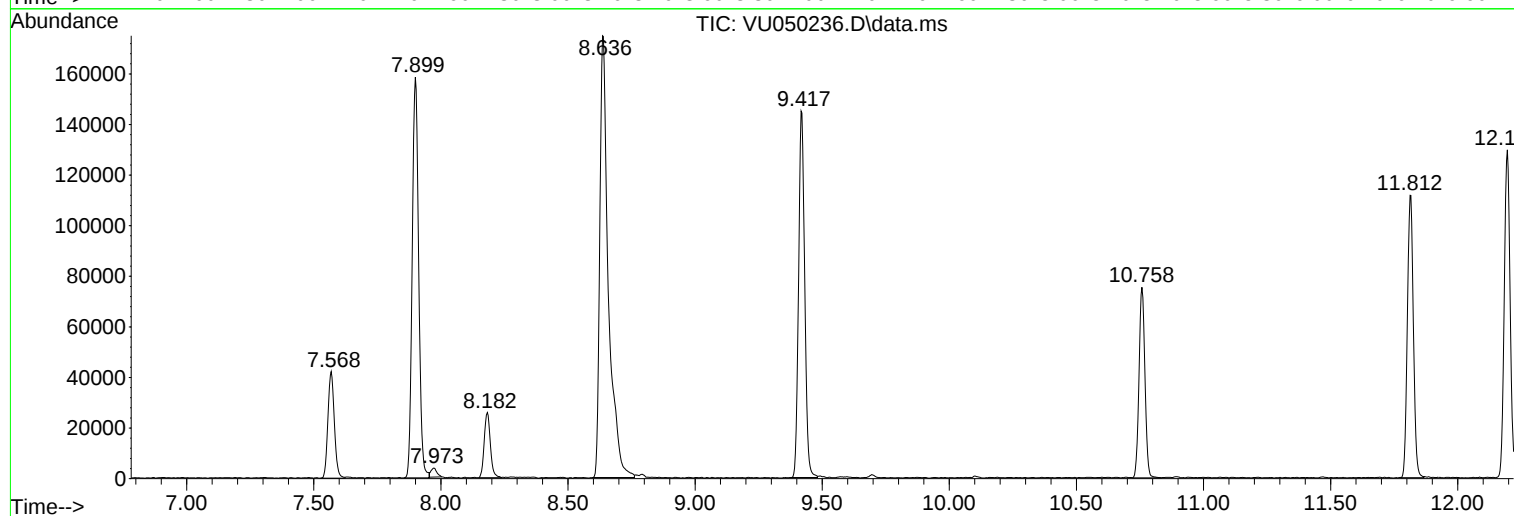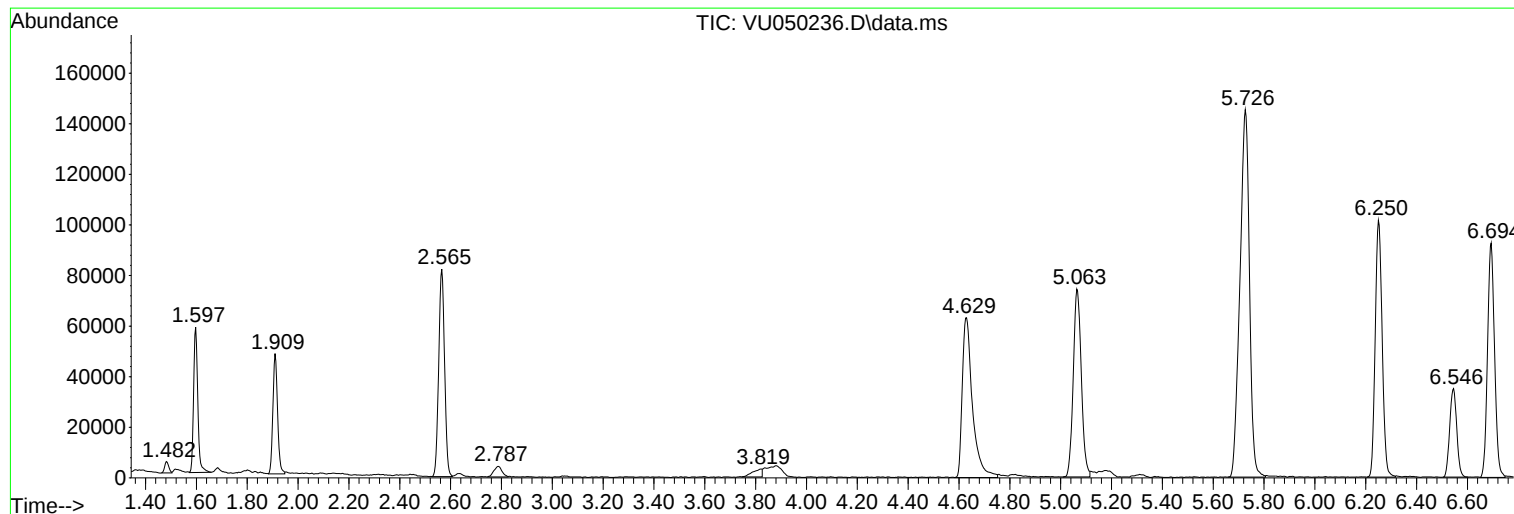

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050236.D
Acq On : 11 Aug 2022 17:33
Operator : SY/MD
Sample : N4160-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050236.D
Acq On : 11 Aug 2022 17:33
Operator : SY/MD
Sample : N4160-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc