

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050257.D
 Acq On : 12 Aug 2022 03:24
 Operator : SY/MD
 Sample : N4161-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGBZ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	52807	58639	13.91%	1.779%
2	1.912	169	178	193	rBV	44378	56349	13.37%	1.710%
3	2.565	367	381	394	rBV	73966	118326	28.08%	3.590%
4	3.829	751	774	775	rBV	2675	5982	1.42%	0.181%
5	3.870	776	787	814	rVB2	7560	27800	6.60%	0.843%
6	4.665	1012	1034	1070	rBV3	130843	400266	94.98%	12.143%
7	5.063	1143	1158	1175	rBV	69595	153060	36.32%	4.643%
8	5.314	1223	1236	1252	rVB2	23223	52766	12.52%	1.601%
9	5.726	1344	1364	1390	rBV2	136990	357330	84.79%	10.841%
10	6.250	1513	1527	1545	rBV	106825	202081	47.95%	6.131%
11	6.542	1604	1618	1637	rBV	71944	134933	32.02%	4.094%
12	6.690	1650	1664	1682	rBV	87226	171331	40.66%	5.198%
13	7.568	1925	1937	1952	rBV	35981	63286	15.02%	1.920%
14	7.899	2027	2040	2055	rBV	142287	251682	59.72%	7.635%
15	7.970	2055	2062	2073	rVB	5414	9666	2.29%	0.293%
16	8.179	2113	2127	2141	rBV2	23423	41932	9.95%	1.272%
17	8.639	2258	2270	2312	rBV6	154590	421414	100.00%	12.785%
18	9.417	2500	2512	2531	rBV	154223	257906	61.20%	7.824%
19	10.758	2916	2929	2946	rBV	75792	120496	28.59%	3.656%
20	11.812	3245	3257	3271	rBV	119022	194028	46.04%	5.886%
21	12.192	3364	3375	3393	rBV	120597	196950	46.74%	5.975%




Sum of corrected areas: 3296223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050257.D
Acq On : 12 Aug 2022 03:24
Operator : SY/MD
Sample : N4161-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

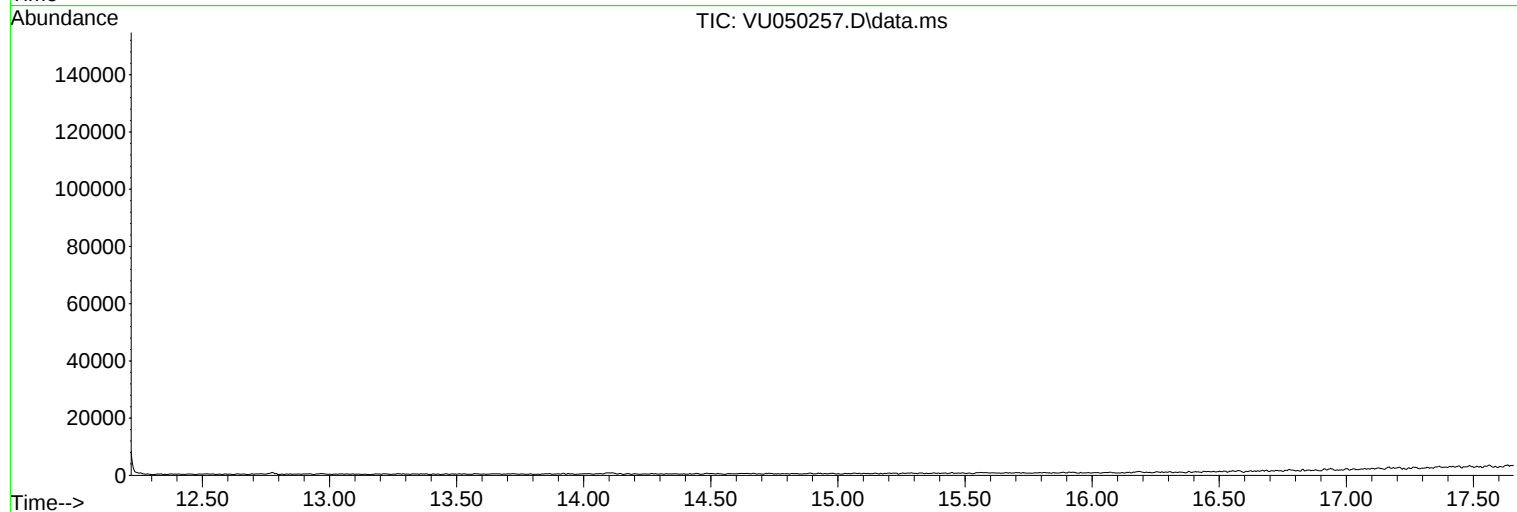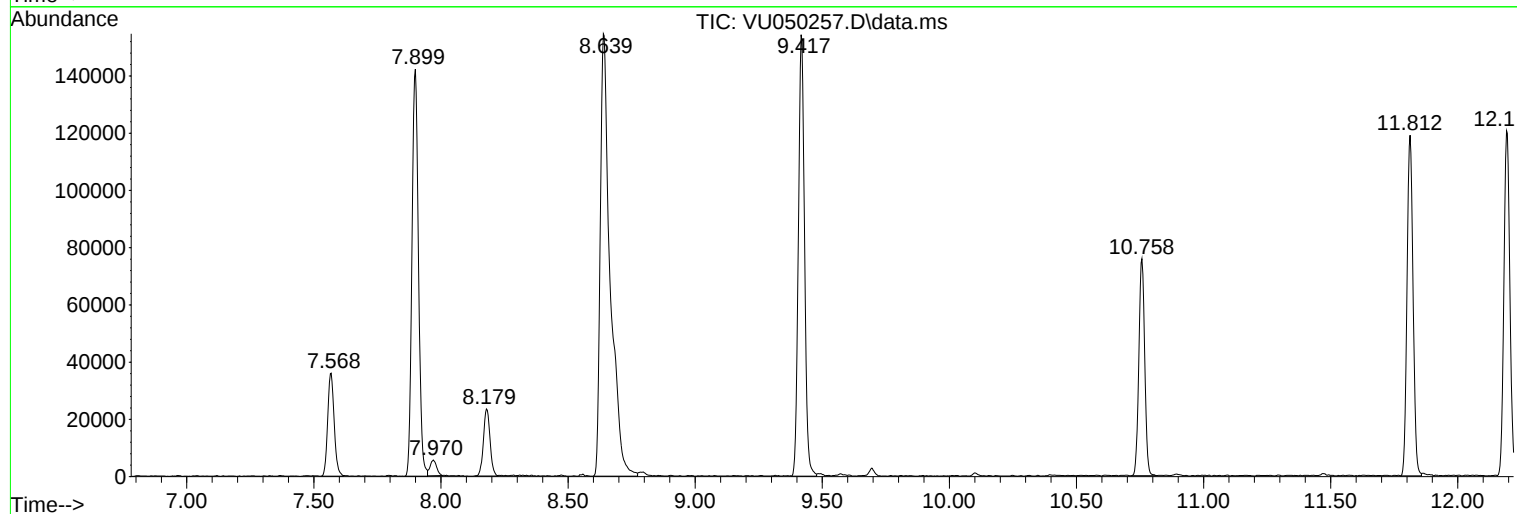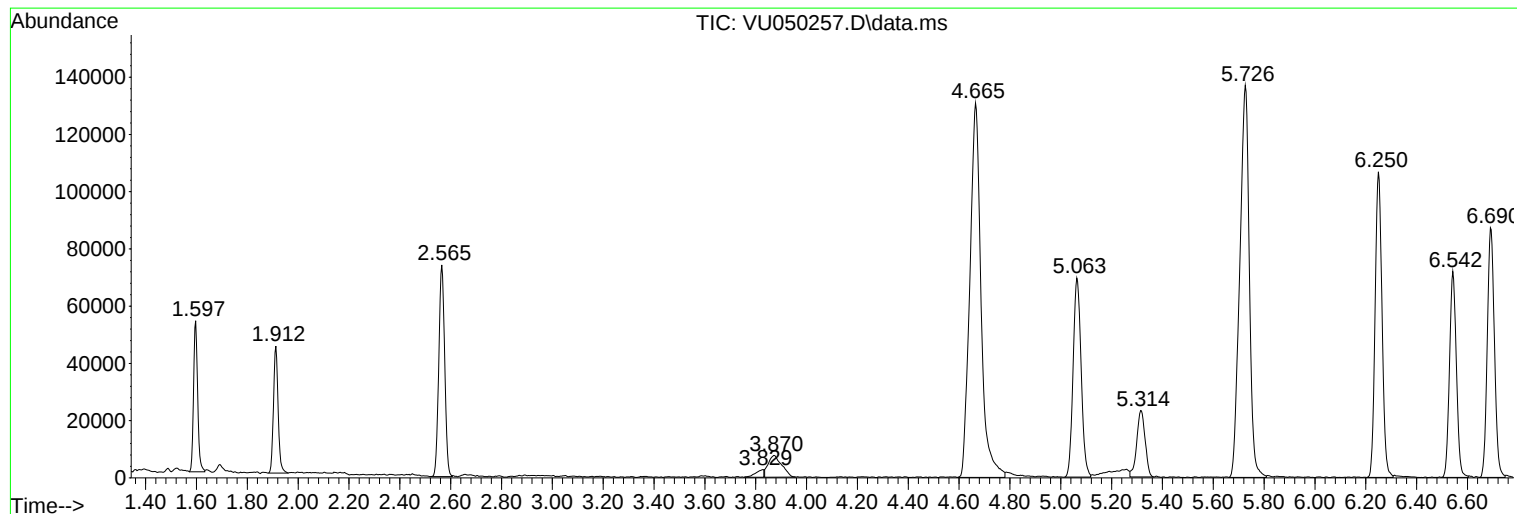

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050257.D
Acq On : 12 Aug 2022 03:24
Operator : SY/MD
Sample : N4161-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050257.D
Acq On : 12 Aug 2022 03:24
Operator : SY/MD
Sample : N4161-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGBZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc