

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050282.D
 Acq On : 12 Aug 2022 15:17
 Operator : SY/MD
 Sample : N4072-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUT7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	97	rVB	47973	53958	13.25%	1.959%
2	1.909	169	177	189	rBV	39858	51170	12.57%	1.858%
3	2.565	367	381	394	rBV	67384	106229	26.09%	3.857%
4	2.636	394	403	416	rVB2	2406	4254	1.04%	0.154%
5	2.777	436	447	463	rBV3	3107	7800	1.92%	0.283%
6	3.851	753	781	783	rBV	4606	14076	3.46%	0.511%
7	4.626	1010	1022	1062	rBV	61376	168965	41.50%	6.135%
8	5.063	1144	1158	1176	rBV	67788	148914	36.58%	5.407%
9	5.726	1344	1364	1385	rBV2	129467	340494	83.64%	12.363%
10	6.250	1513	1527	1546	rBV	101964	194810	47.85%	7.074%
11	6.694	1646	1665	1687	rBV	86271	166822	40.98%	6.057%
12	7.568	1925	1937	1952	rBV	38626	67612	16.61%	2.455%
13	7.899	2027	2040	2057	rBV	137232	237954	58.45%	8.640%
14	8.179	2114	2127	2143	rBV	22880	38672	9.50%	1.404%
15	8.639	2257	2270	2309	rBV5	157298	407108	100.00%	14.782%
16	9.417	2501	2512	2531	rBV	147068	244001	59.94%	8.860%
17	9.703	2593	2601	2613	rBV5	3632	5552	1.36%	0.202%
18	10.758	2917	2929	2947	rVB	72060	115361	28.34%	4.189%
19	11.812	3244	3257	3273	rBV	117306	188701	46.35%	6.852%
20	12.195	3364	3376	3395	rBV	118461	191596	47.06%	6.957%




Sum of corrected areas: 2754049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050282.D
Acq On : 12 Aug 2022 15:17
Operator : SY/MD
Sample : N4072-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

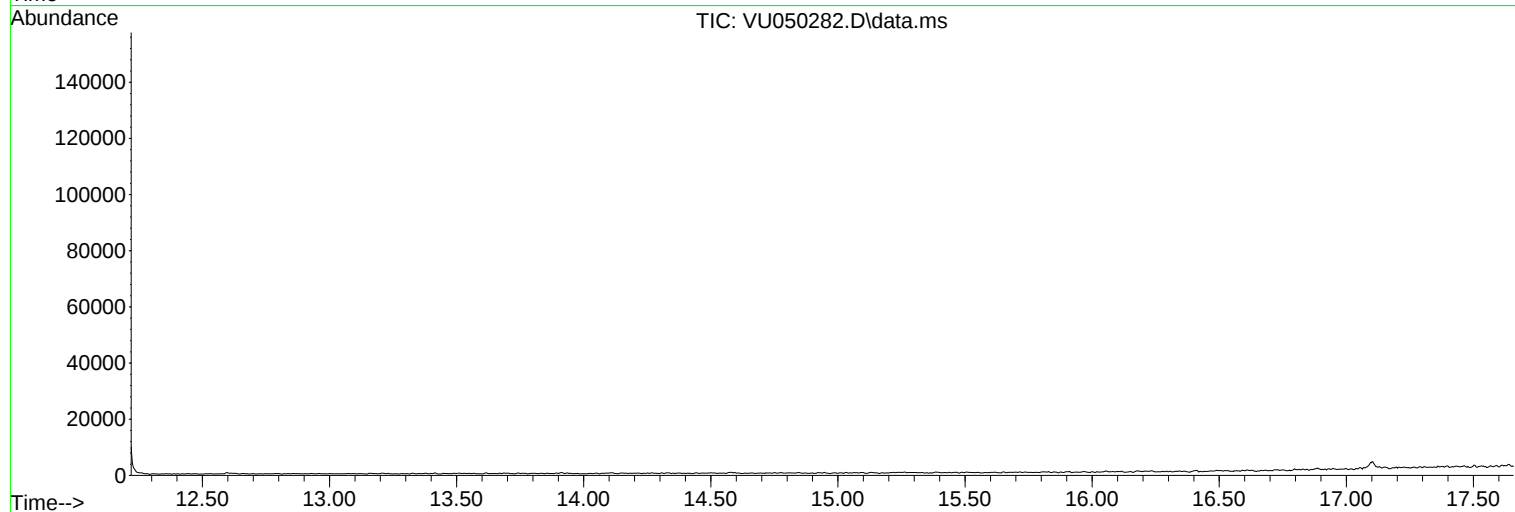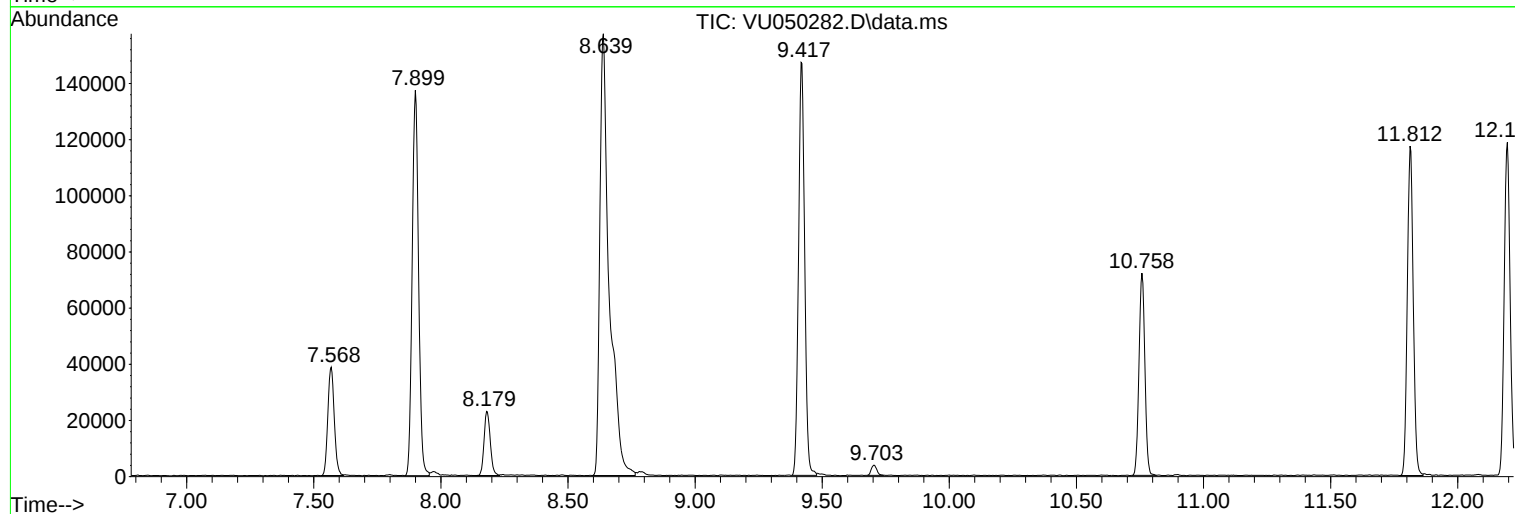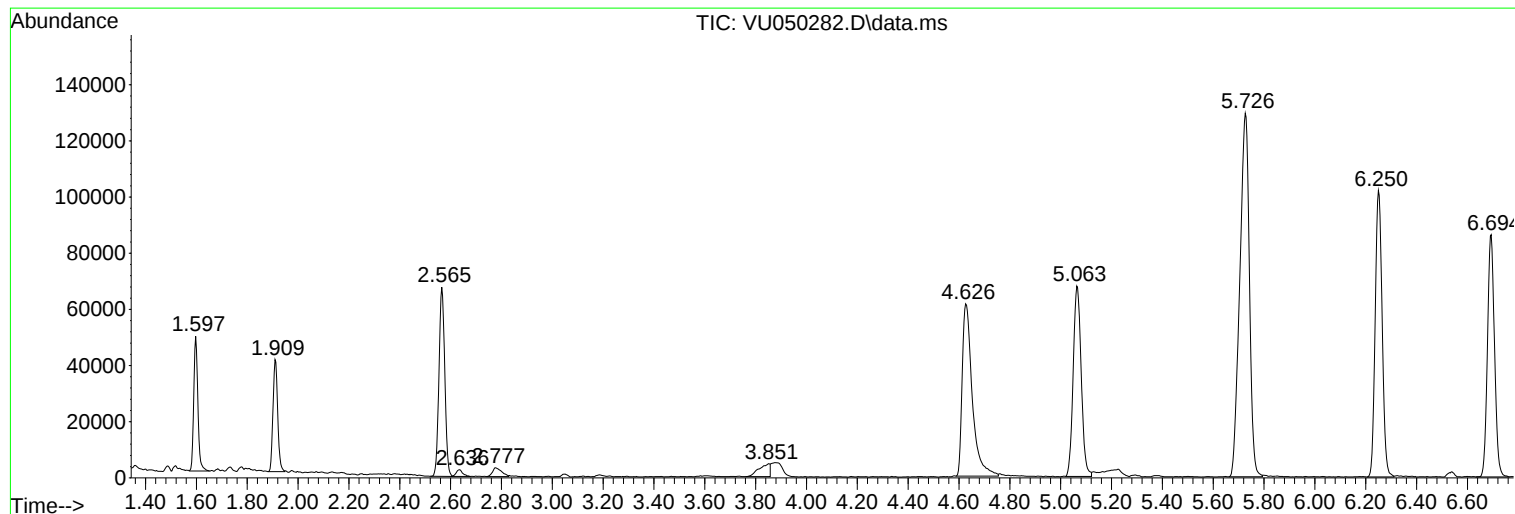

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050282.D
Acq On : 12 Aug 2022 15:17
Operator : SY/MD
Sample : N4072-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050282.D
Acq On : 12 Aug 2022 15:17
Operator : SY/MD
Sample : N4072-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
