

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050287.D
 Acq On : 12 Aug 2022 18:00
 Operator : SY/MD
 Sample : N4072-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUU2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	93	rBV	52952	60654	14.48%	2.221%
2	1.768	128	133	143	rBV2	4506	5423	1.29%	0.199%
3	1.909	169	177	190	rVB	40125	50904	12.15%	1.864%
4	2.562	368	380	394	rVB	70715	113211	27.02%	4.145%
5	3.809	750	768	769	rBV	2885	5890	1.41%	0.216%
6	4.649	1015	1029	1074	rBV2	42519	173045	41.31%	6.335%
7	5.063	1140	1158	1177	rBV	64967	145066	34.63%	5.311%
8	5.726	1344	1364	1392	rBV2	124690	323888	77.31%	11.857%
9	6.250	1514	1527	1556	rBV	103261	198594	47.40%	7.270%
10	6.694	1652	1665	1686	rBV	80223	157509	37.60%	5.766%
11	7.568	1925	1937	1952	rBV2	35270	60891	14.53%	2.229%
12	7.899	2027	2040	2056	rBV	130104	225359	53.79%	8.250%
13	8.182	2117	2128	2143	rBV	21648	36021	8.60%	1.319%
14	8.642	2258	2271	2308	rBV3	164196	418942	100.00%	15.337%
15	8.793	2308	2318	2328	rVB7	3500	6484	1.55%	0.237%
16	9.420	2500	2513	2536	rBV	149637	248540	59.33%	9.099%
17	10.758	2917	2929	2948	rVB	70569	113423	27.07%	4.152%
18	11.812	3245	3257	3281	rBV	118861	194068	46.32%	7.105%
19	12.195	3365	3376	3393	rBV	113220	184719	44.09%	6.763%
20	12.889	3585	3592	3601	rBV4	6290	8882	2.12%	0.325%




Sum of corrected areas: 2731513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050287.D
Acq On : 12 Aug 2022 18:00
Operator : SY/MD
Sample : N4072-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

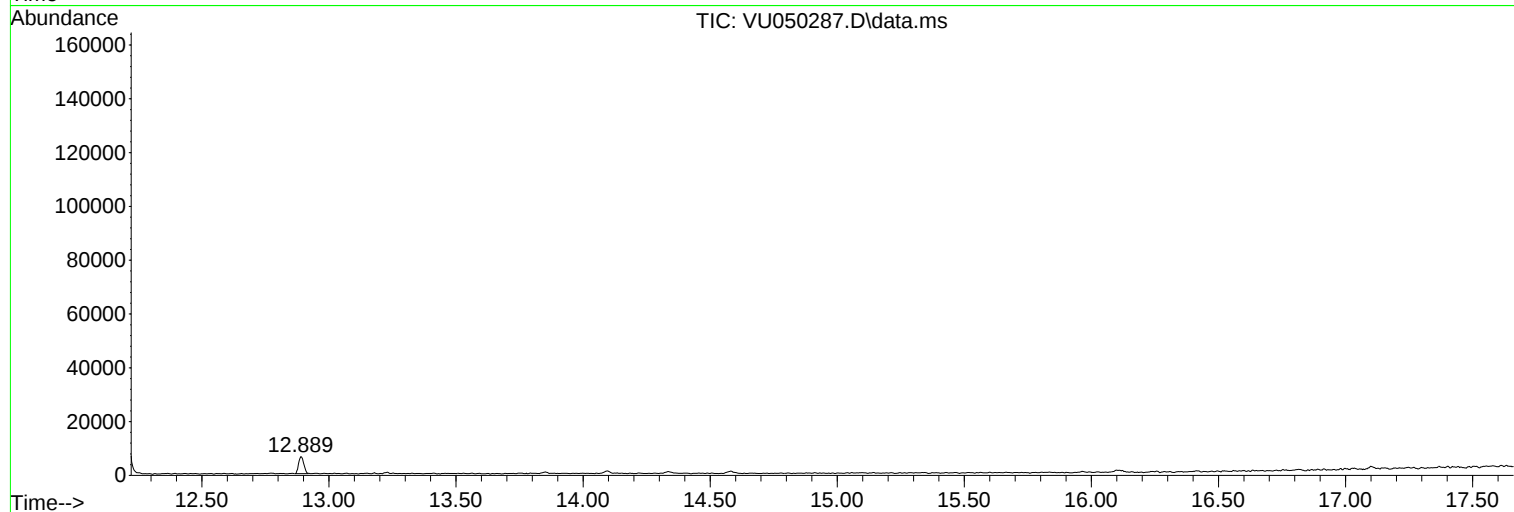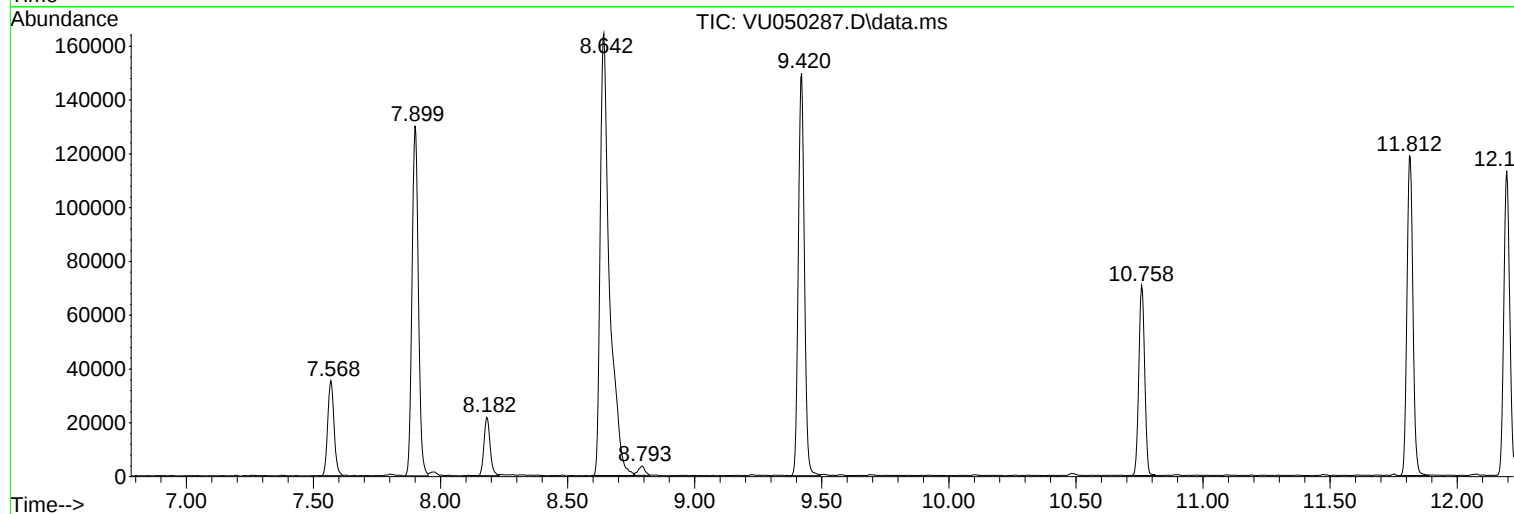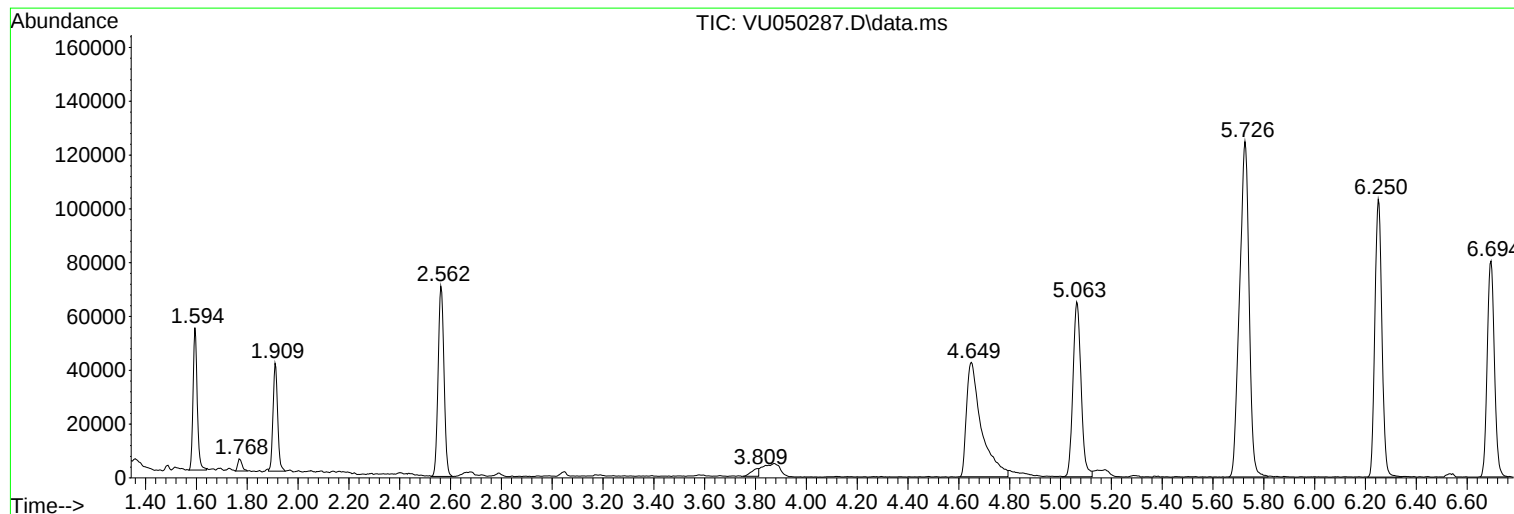

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050287.D
Acq On : 12 Aug 2022 18:00
Operator : SY/MD
Sample : N4072-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
Data File : VU050287.D
Acq On : 12 Aug 2022 18:00
Operator : SY/MD
Sample : N4072-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUU2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc