


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081122\
 Data File : VU050224.D
 Acq On : 11 Aug 2022 09:00
 Operator : SY/MD
 Sample : BFB103
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB103

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sun Aug 14 01:24:58 2022

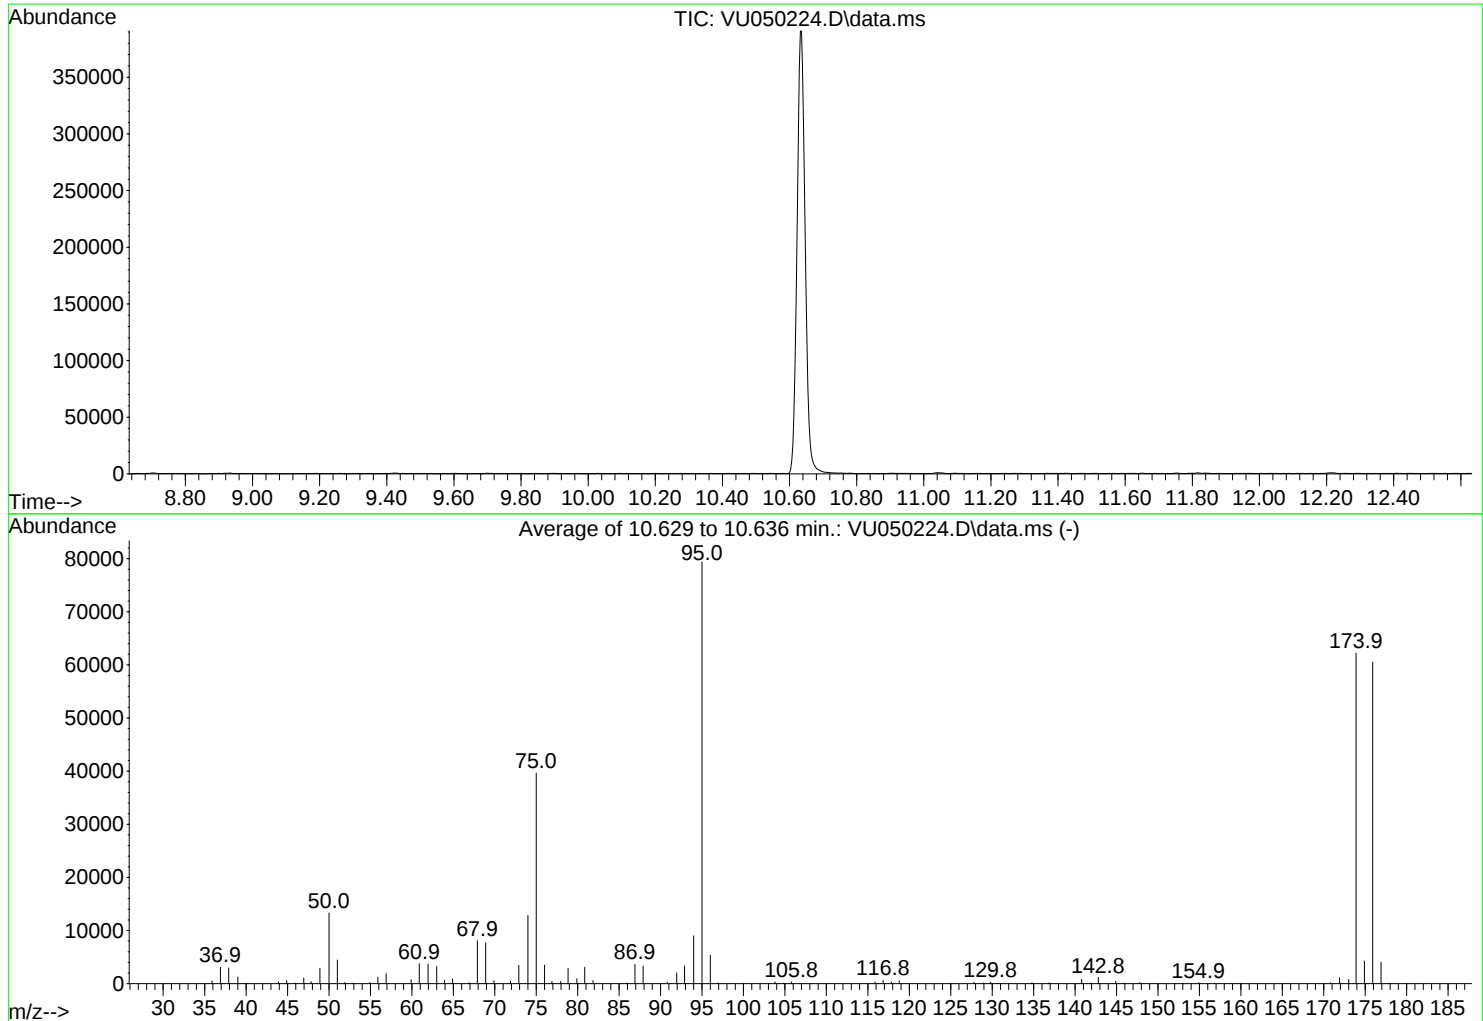

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	13317	PASS
75	95	30	80	49.9	39603	PASS
95	95	100	100	100.0	79395	PASS
96	95	5	9	6.8	5363	PASS
173	174	0.00	2	1.3	825	PASS
174	95	50	120	78.4	62213	PASS
175	174	5	9	6.8	4252	PASS
176	174	95	101	97.3	60541	PASS
177	176	5	9	6.7	4071	PASS

m/z	Abundance
39.80	120.0
43.90	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	482.0
36.90	2969.0
37.90	2800.0
39.00	1277.0
40.00	150.0
43.90	606.0
44.90	527.0
45.90	115.0
46.90	992.0
47.80	355.0
48.90	2842.0
50.00	12649.0
51.00	4159.0
51.90	170.0
54.90	201.0
55.90	1244.0
56.90	1818.0
59.90	750.0
60.90	3590.0
62.00	3597.0
63.00	3036.0
63.90	586.0
64.90	823.0
66.90	198.0
67.90	7636.0
68.90	7336.0
69.90	508.0
71.90	431.0
72.90	3253.0
74.00	12287.0
75.00	37272.0
76.00	3210.0
76.90	425.0
77.90	426.0
78.80	2762.0
79.90	782.0
80.90	2926.0
81.90	581.0
86.90	3424.0
87.90	3134.0
90.80	291.0
91.90	1869.0
92.90	3141.0
94.00	8442.0
95.00	75296.0
96.00	5097.0
96.90	115.0
103.80	333.0
105.80	352.0
115.90	275.0
116.90	603.0
117.90	258.0
118.80	508.0
127.80	228.0
128.90	103.0
129.80	261.0
134.80	160.0
136.90	147.0
140.80	825.0
141.90	104.0
142.80	1104.0
144.90	429.0
147.80	210.0
154.90	172.0
156.90	109.0
170.80	178.0
171.90	1012.0
173.00	827.0
173.90	57696.0
174.90	4003.0
175.90	55784.0
176.90	3913.0
177.80	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	532.0
36.90	3146.0
37.90	3039.0
39.00	1303.0
39.90	163.0
43.90	574.0
44.90	570.0
45.90	133.0
46.90	1098.0
47.80	386.0
48.90	2965.0
50.00	13711.0
51.00	4648.0
51.90	231.0
52.90	130.0
54.90	239.0
55.90	1299.0
56.90	1981.0
59.90	803.0
60.90	3848.0
62.00	3790.0
63.00	3337.0
63.90	625.0
64.90	906.0
66.90	212.0
67.90	8424.0
68.90	7951.0
69.90	588.0
71.90	473.0
72.90	3552.0
74.00	13191.0
75.00	40720.0
76.00	3562.0
76.90	449.0
77.90	394.0
78.80	2992.0
79.90	976.0
80.80	3163.0
81.80	605.0
85.90	141.0
86.90	3773.0
87.90	3421.0
90.80	293.0
92.00	2049.0
92.90	3382.0
94.00	9219.0
95.00	81792.0
96.00	5512.0
96.90	148.0
103.80	347.0
104.80	112.0
105.80	354.0
115.80	306.0
116.80	631.0
117.80	327.0
118.80	549.0
127.80	281.0
128.90	138.0
129.80	313.0
130.80	113.0
134.80	175.0
136.80	155.0
140.80	863.0
141.90	108.0
142.80	1194.0
144.90	445.0
145.90	111.0
147.80	227.0
154.90	180.0
156.80	128.0
170.80	199.0
171.90	1099.0
173.00	864.0
173.90	64008.0
174.90	4362.0
175.90	62432.0
176.90	4209.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	491.0
36.90	3142.0
37.90	2986.0
39.00	1264.0
39.90	139.0
43.90	568.0
44.90	586.0
45.90	146.0
47.00	1035.0
47.90	393.0
48.90	2860.0
50.00	13592.0
51.00	4576.0
51.90	248.0
52.90	129.0
54.90	225.0
55.90	1191.0
56.90	1910.0
59.90	726.0
60.90	3743.0
61.90	3743.0
63.00	3290.0
64.00	588.0
64.90	938.0
66.90	217.0
67.90	8157.0
68.90	7798.0
69.90	593.0
71.90	482.0
72.90	3515.0
74.00	12983.0
75.00	40816.0
76.00	3698.0
76.90	444.0
78.00	360.0
78.90	2957.0
79.90	1008.0
80.80	3143.0
81.80	595.0
85.90	178.0
86.90	3687.0
87.90	3433.0
90.80	269.0
92.00	2178.0
92.90	3461.0
94.00	9317.0
95.00	81096.0
96.00	5480.0
96.90	163.0
103.80	292.0
104.80	127.0
105.80	321.0
115.80	333.0
116.80	602.0
117.80	368.0
118.80	565.0
127.80	286.0
128.90	148.0
129.80	322.0
130.80	115.0
134.80	182.0
136.80	132.0
140.80	761.0
141.90	109.0
142.80	1207.0
144.90	382.0
145.90	141.0
147.80	208.0
154.90	164.0
156.80	144.0
158.80	109.0
170.80	208.0
171.90	1110.0
173.00	784.0
173.90	64936.0
174.90	4392.0
175.90	63408.0
176.90	4090.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103