

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081220\
 Data File : VU039838.D
 Acq On : 12 Aug 2020 11:07
 Operator : SY/MD
 Sample : VU0812WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.752	436	439	443	rVB4	808	685	1.24%	0.309%
2	2.793	447	452	453	rBV4	849	725	1.31%	0.327%
3	3.057	529	534	544	rVB4	3915	6524	11.81%	2.945%
4	3.202	571	579	588	rBV5	2178	4428	8.02%	1.999%
5	3.350	620	625	628	rBV5	584	665	1.20%	0.300%
6	3.707	732	736	741	rVB5	580	574	1.04%	0.259%
7	4.070	846	849	855	rBV4	573	731	1.32%	0.330%
8	4.404	949	953	955	rBV4	788	615	1.11%	0.278%
9	4.716	1032	1050	1072	rBV2	10257	36885	66.77%	16.650%
10	4.896	1101	1106	1107	rBV2	1009	776	1.40%	0.350%
11	5.263	1215	1220	1222	rBV3	557	579	1.05%	0.261%
12	5.295	1227	1230	1237	rVB4	924	1015	1.84%	0.458%
13	5.395	1259	1261	1265	rVB4	926	680	1.23%	0.307%
14	6.125	1476	1488	1509	rVB2	28477	55245	100.00%	24.937%
15	6.292	1538	1540	1546	rVB5	681	565	1.02%	0.255%
16	7.819	2004	2015	2022	rBV4	1808	3051	5.52%	1.377%
17	7.906	2032	2042	2046	rBV3	594	678	1.23%	0.306%
18	8.350	2176	2180	2186	rBV4	584	575	1.04%	0.260%
19	8.700	2279	2289	2302	rBV4	1727	2988	5.41%	1.349%
20	8.938	2353	2363	2380	rVB	2767	4748	8.59%	2.143%
21	10.632	2876	2890	2901	rVB2	19405	30937	56.00%	13.965%
22	10.896	2968	2972	2975	rBV4	661	707	1.28%	0.319%
23	11.092	3028	3033	3043	rVB4	589	1135	2.05%	0.512%
24	11.636	3199	3202	3213	rVV4	480	789	1.43%	0.356%
25	11.748	3231	3237	3241	rVB4	637	698	1.26%	0.315%
26	11.790	3248	3250	3257	rVB2	569	560	1.01%	0.253%
27	11.835	3257	3264	3270	rBV5	1157	1620	2.93%	0.731%
28	12.189	3364	3374	3388	rBV	27208	44988	81.43%	20.307%
29	12.677	3522	3526	3534	rBV3	450	615	1.11%	0.278%
30	12.767	3550	3554	3559	rVB2	677	648	1.17%	0.293%
31	13.828	3878	3884	3894	rVV5	2795	3637	6.58%	1.642%
32	14.079	3952	3962	3969	rBV	3731	5650	10.23%	2.550%
33	14.317	4029	4036	4045	rVB4	2973	4115	7.45%	1.857%
34	16.156	4601	4608	4615	rBV4	675	1098	1.99%	0.496%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081220\
Data File : VU039838.D
Acq On : 12 Aug 2020 11:07
Operator : SY/MD
Sample : VU0812WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK18

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	16.867	4825	4829	4836	rbV4	767	1051	1.90%	0.474%
36	17.613	5056	5061	5065	rbV5	448	555	1.00%	0.251%


Sum of corrected areas: 221535

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081220\
Data File : VU039838.D
Acq On : 12 Aug 2020 11:07
Operator : SY/MD
Sample : VU0812WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK18

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

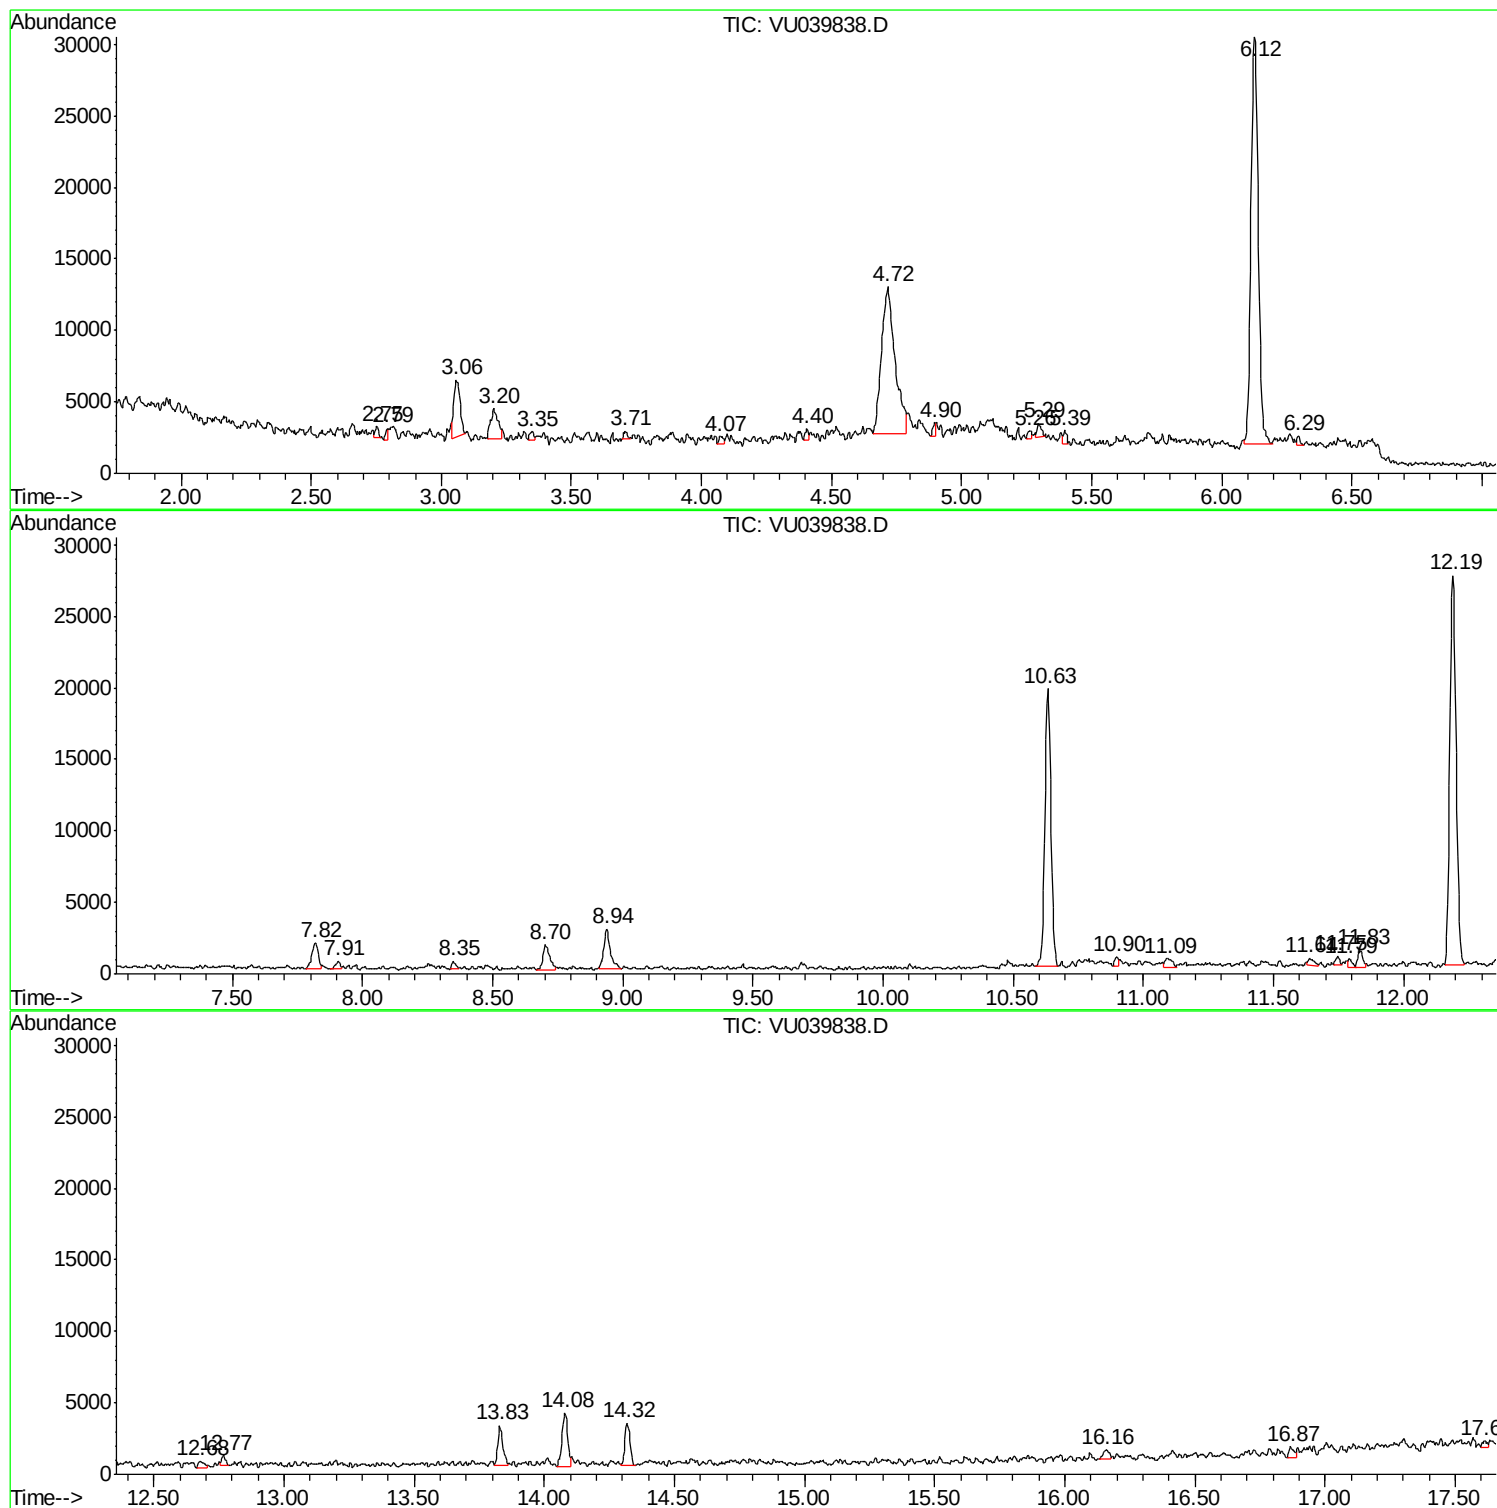

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU081220\
Data File : VU039838.D
Acq On : 12 Aug 2020 11:07
Operator : SY/MD
Sample : VU0812WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK18

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU081220\
Data File : VU039838.D
Acq On : 12 Aug 2020 11:07
Operator : SY/MD
Sample : VU0812WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK18

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc