
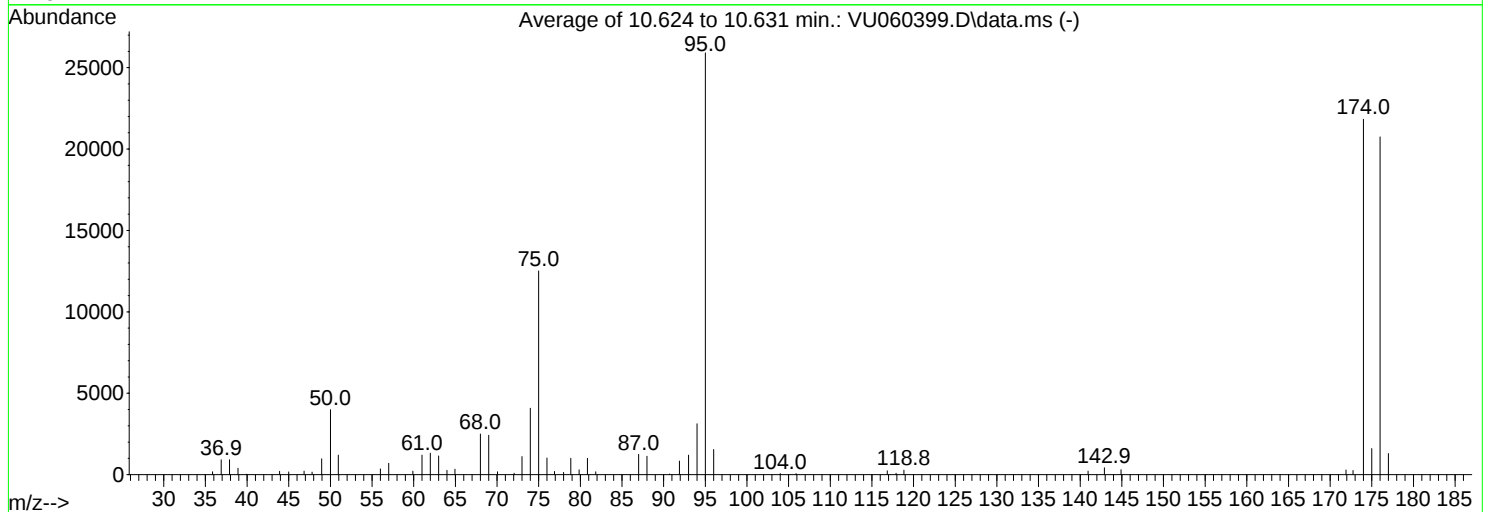


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081224\
Data File : VU060399.D
Acq On : 12 Aug 2024 11:35
Operator : MD/SY
Sample : BFB183
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB183

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Aug 13 16:28:40 2024

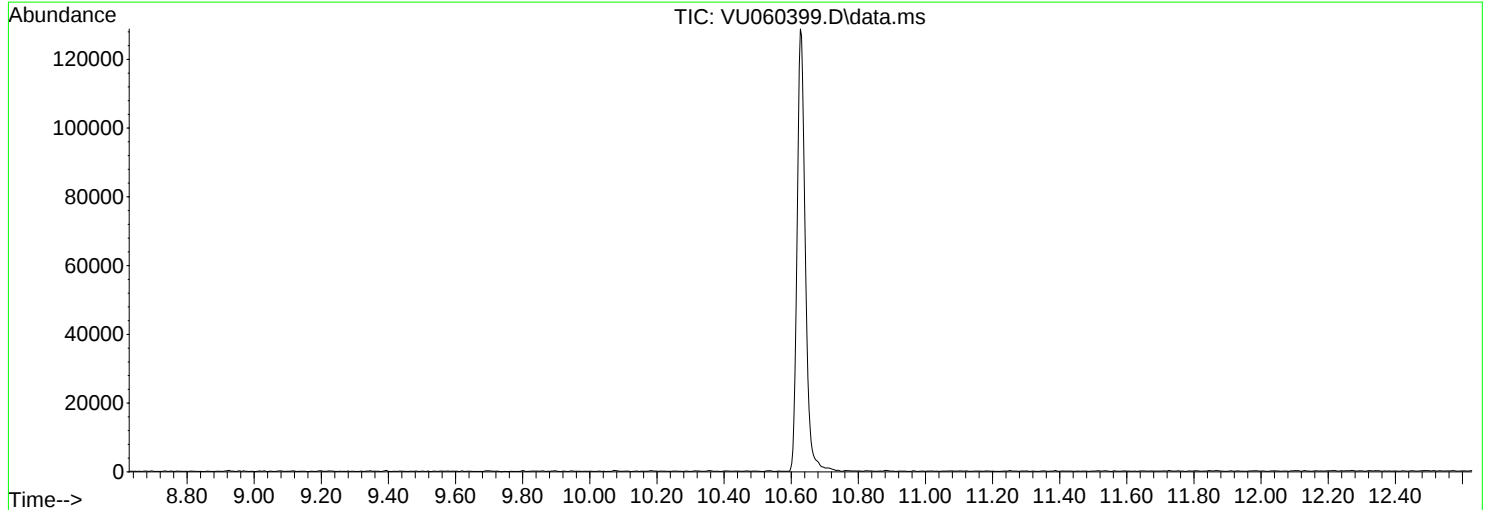

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	3992	PASS
75	95	30	80	48.3	12507	PASS
95	95	100	100	100.0	25909	PASS
96	95	5	9	6.0	1546	PASS
173	174	0.00	2	1.2	256	PASS
174	95	50	120	84.3	21829	PASS
175	174	5	9	7.3	1604	PASS
176	174	95	101	95.1	20749	PASS
177	176	5	9	6.2	1295	PASS

m/z	Abundance
43.90	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.80	152.0
36.90	909.0
37.90	818.0
38.90	392.0
39.90	101.0
43.90	430.0
45.00	165.0
46.80	169.0
47.70	159.0
49.00	940.0
50.00	3879.0
50.90	1094.0
56.00	331.0
57.00	711.0
59.90	216.0
61.00	1176.0
62.00	1179.0
63.00	1047.0
64.00	259.0
64.90	350.0
68.00	2383.0
69.00	2325.0
70.10	174.0
73.00	1110.0
74.00	3893.0
75.00	12155.0
76.00	923.0
76.90	226.0
78.10	113.0
78.90	1006.0
79.90	300.0
80.90	976.0
81.90	139.0
87.00	1191.0
88.00	1019.0
91.90	879.0
93.00	1264.0
94.00	2948.0
95.00	24312.0
96.00	1463.0
104.00	109.0
105.90	114.0
116.90	218.0
118.90	269.0
141.00	191.0
142.90	326.0
144.90	265.0
171.90	287.0
172.80	392.0
174.00	20712.0
175.00	1558.0
176.00	19096.0
177.00	1186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.80	178.0
36.90	932.0
37.90	952.0
38.90	423.0
43.90	396.0
45.00	181.0
46.90	218.0
47.80	161.0
49.00	995.0
50.00	4104.0
51.00	1215.0
56.00	376.0
57.00	727.0
59.90	215.0
61.00	1259.0
62.00	1375.0
63.00	1206.0
64.00	282.0
64.90	352.0
68.00	2580.0
69.00	2460.0
70.10	176.0
72.00	127.0
73.00	1138.0
74.00	4183.0
75.00	12957.0
76.00	1066.0
76.90	218.0
78.00	134.0
78.80	1043.0
79.90	294.0
80.90	1001.0
81.90	184.0
87.00	1296.0
88.00	1170.0
91.90	864.0
93.00	1229.0
94.00	3250.0
95.00	26848.0
96.00	1592.0
104.00	108.0
105.90	102.0
116.90	255.0
117.90	112.0
118.90	309.0
141.00	228.0
142.90	426.0
144.90	325.0
171.90	278.0
172.70	375.0
174.00	22528.0
175.00	1644.0
176.00	21408.0
177.00	1337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	217.0
36.90	903.0
37.90	971.0
38.90	373.0
43.90	356.0
45.00	167.0
46.90	260.0
47.90	146.0
48.90	977.0
50.00	3992.0
51.00	1293.0
56.00	359.0
57.00	661.0
59.90	220.0
61.00	1149.0
62.00	1392.0
63.00	1190.0
64.00	260.0
65.00	300.0
68.00	2526.0
69.00	2478.0
69.90	188.0
72.10	135.0
73.00	1076.0
74.00	4171.0
75.00	12410.0
76.00	1081.0
76.90	153.0
77.90	161.0
78.80	962.0
79.80	280.0
80.80	1020.0
81.80	218.0
87.00	1247.0
88.00	1207.0
90.70	127.0
91.90	767.0
93.00	1103.0
94.00	3183.0
95.00	26568.0
96.00	1582.0
116.80	243.0
117.90	157.0
118.80	263.0
140.90	238.0
142.90	528.0
144.90	313.0
171.90	292.0
174.00	22248.0
175.00	1611.0
176.00	21744.0
177.00	1361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183