

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081318\
 Data File : VU026055.D
 Acq On : 13 Aug 2018 09:43
 Operator : MD/SY
 Sample : VU0813WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 14 01:14:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 14 01:13:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	301360	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	278092	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	123458	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	104478	47.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.86%
7) Chloroethane-d5	1.68	69	84488	48.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.76%
11) 1,1-Dichloroethene-d2	2.27	63	151315	36.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.30%
21) 2-Butanone-d5	4.18	46	152147	82.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.87%
24) Chloroform-d	4.65	84	213943	45.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.31	65	144493	45.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.58%
32) Benzene-d6	5.35	84	422098	48.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.76%
36) 1,2-Dichloropropane-d6	6.33	67	137377	49.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.34%
41) Toluene-d8	7.57	98	393009	47.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.14%
43) trans-1,3-Dichloropropene-	7.85	79	65762	46.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.42%
47) 2-Hexanone-d5	8.31	63	104436	82.29	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.29%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	181535	44.43	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.86%
64) 1,2-Dichlorobenzene-d4	11.86	152	151608	49.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.62%


Target Compounds					Ovalue
13) Acetone	2.32	43	1443	1.265 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081318\
Data File : VU026055.D
Acq On : 13 Aug 2018 09:43
Operator : MD/SY
Sample : VU0813WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 14 01:14:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 14 01:13:22 2018
Response via : Initial Calibration

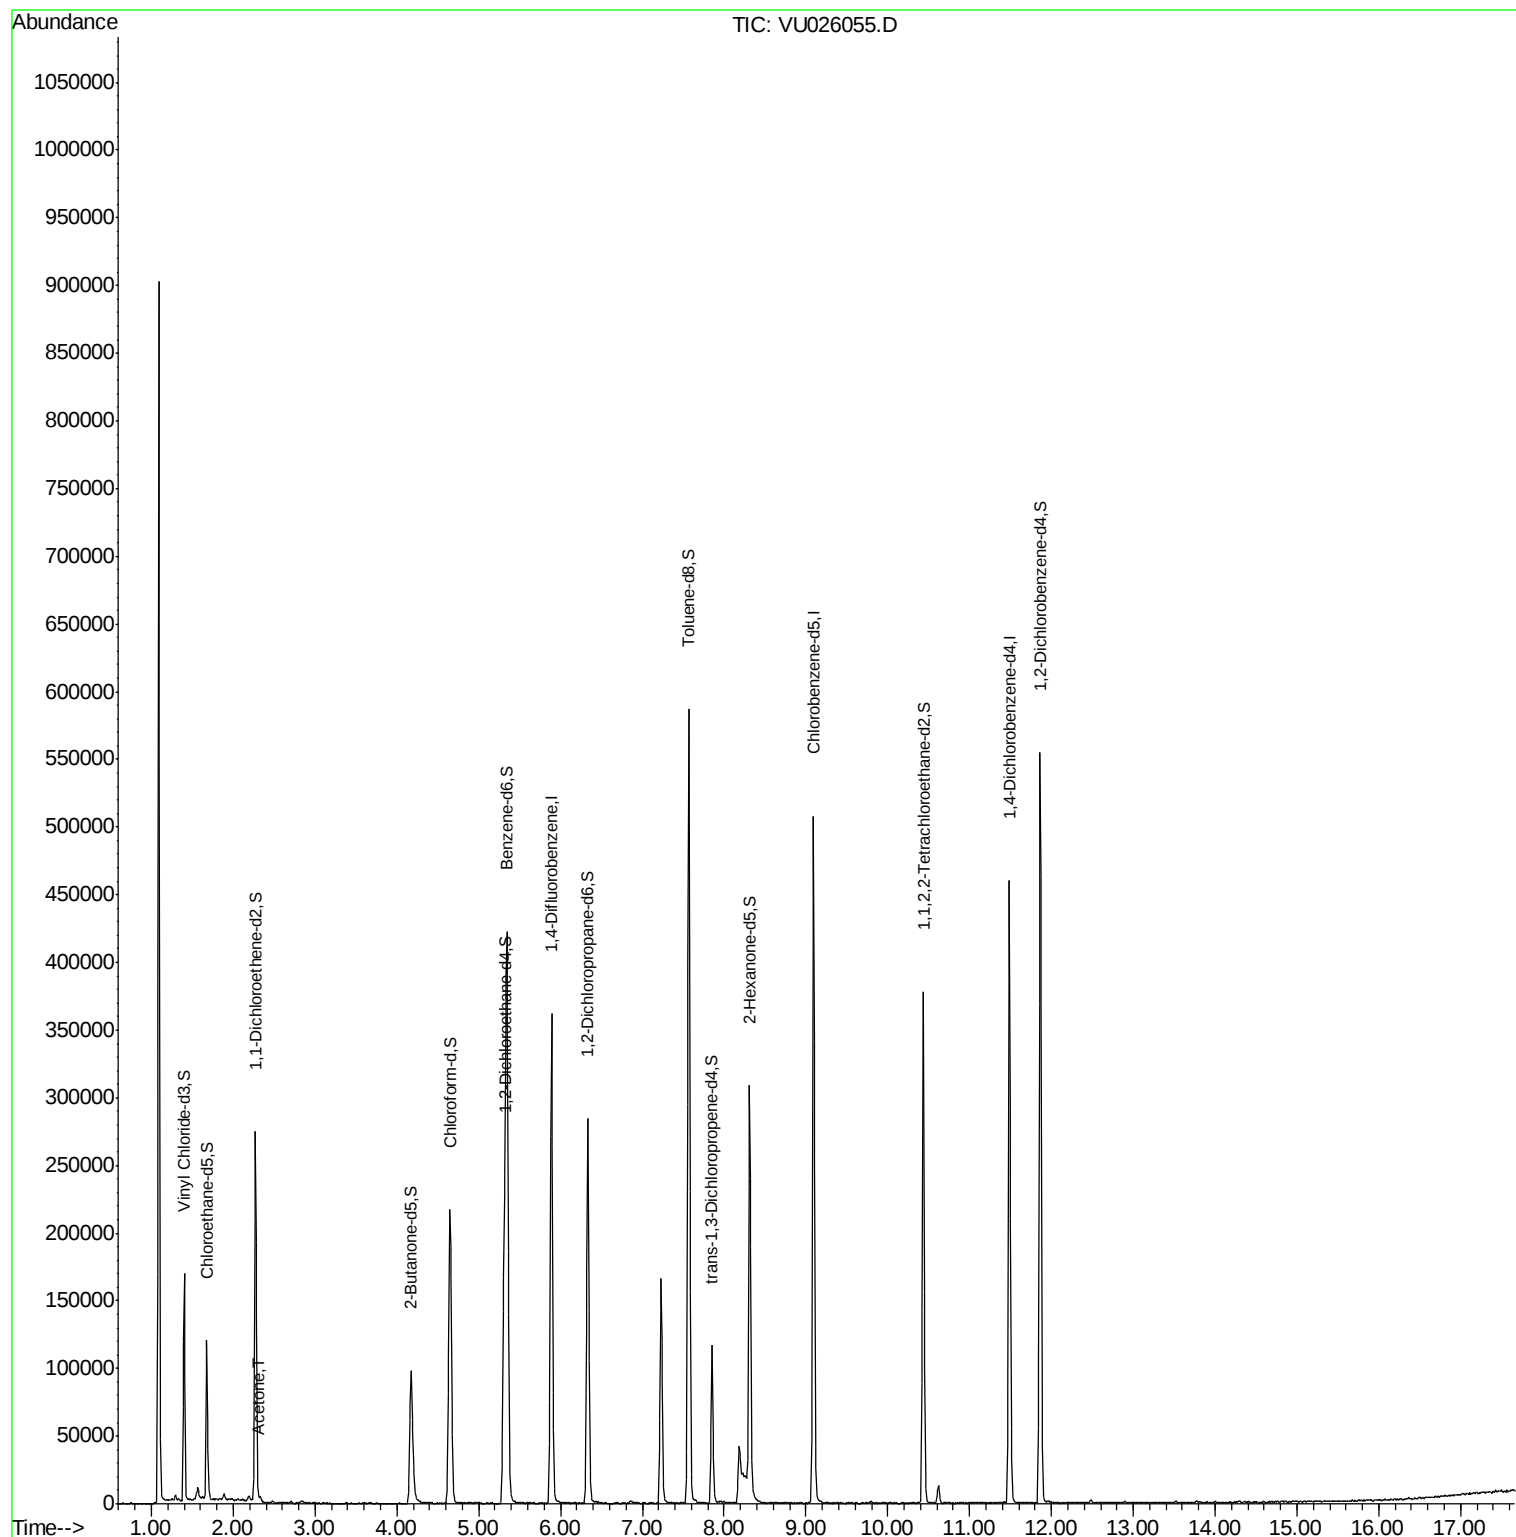

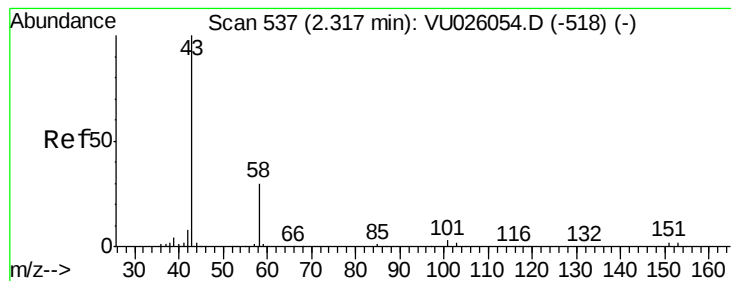

#13

Acetone

Concen: 1.265 ug/L

RT: 2.32 min Scan# 538

Delta R.T. 0.00 min

Lab File: VU026055.D

Acq: 13 Aug 2018 09:43

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 43 Resp: 1443

Ion Ratio Lower Upper

43 100

58 23.4 0.0 61.8

