

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081318\
 Data File : VU026087.D
 Acq On : 13 Aug 2018 23:06
 Operator : MD/SY
 Sample : J4451-13 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 14 02:21:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 14 02:18:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	273285	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	255742	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	109486	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	78358	39.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.46%
7) Chloroethane-d5	1.67	69	67691	42.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.48%
11) 1,1-Dichloroethene-d2	2.27	63	123331	32.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.98%
21) 2-Butanone-d5	4.18	46	136907	82.23	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.23%
24) Chloroform-d	4.65	84	182399	43.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.12%
26) 1,2-Dichloroethane-d4	5.31	65	125260	43.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.54%
32) Benzene-d6	5.35	84	352652	44.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.82%
36) 1,2-Dichloropropane-d6	6.33	67	116685	45.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.82%
41) Toluene-d8	7.57	98	317213	41.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.50%
43) trans-1,3-Dichloropropene-	7.85	79	54655	42.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.44%
47) 2-Hexanone-d5	8.31	63	94619	81.07	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.07%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	160253	42.65	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.30%
64) 1,2-Dichlorobenzene-d4	11.86	152	122203	45.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.56%


Target Compounds					Ovalue
13) Acetone	2.32	43	1362	1.317 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081318\
Data File : VU026087.D
Acq On : 13 Aug 2018 23:06
Operator : MD/SY
Sample : J4451-13 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 14 02:21:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 14 02:18:47 2018
Response via : Initial Calibration

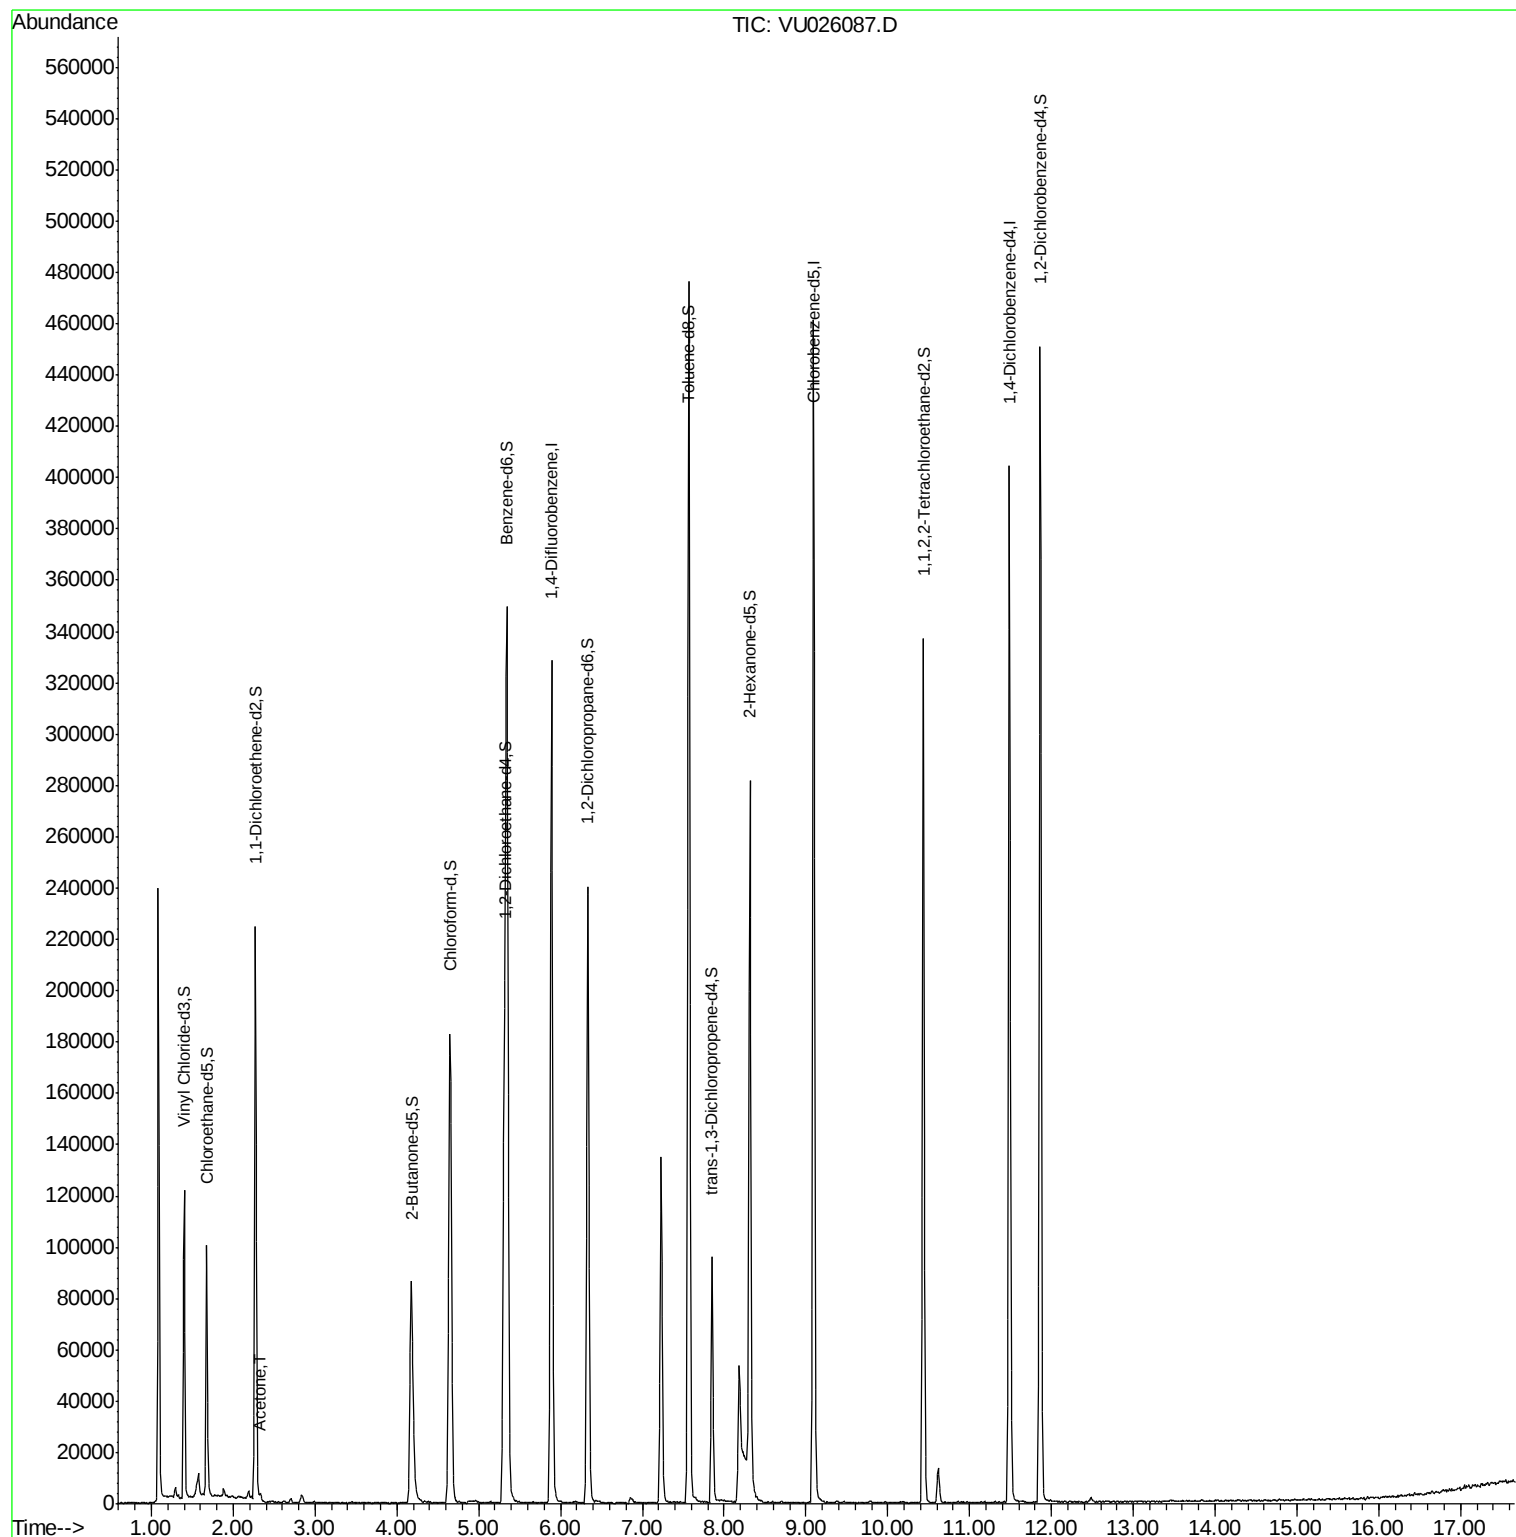

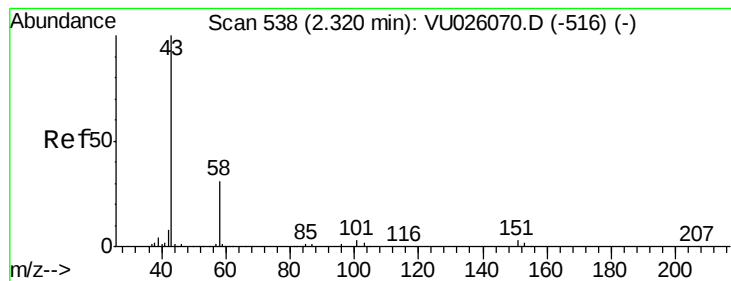

#13
 Acetone
 Concen: 1.317 ug/L
 RT: 2.32 min Scan# 539
 Delta R.T. 0.00 min
 Lab File: VU026087.D
 Acq: 13 Aug 2018 23:06

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion: 43 Resp: 1362
 Ion Ratio Lower Upper
 43 100
 58 23.8 0.0 61.8

