


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081319\
 Data File : VU033774.D
 Acq On : 13 Aug 2019 08:24
 Operator : JC/SP
 Sample : BFB55
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM081319W.M
 Title : VOC Analysis
 Last Update : Wed Aug 14 04:23:45 2019

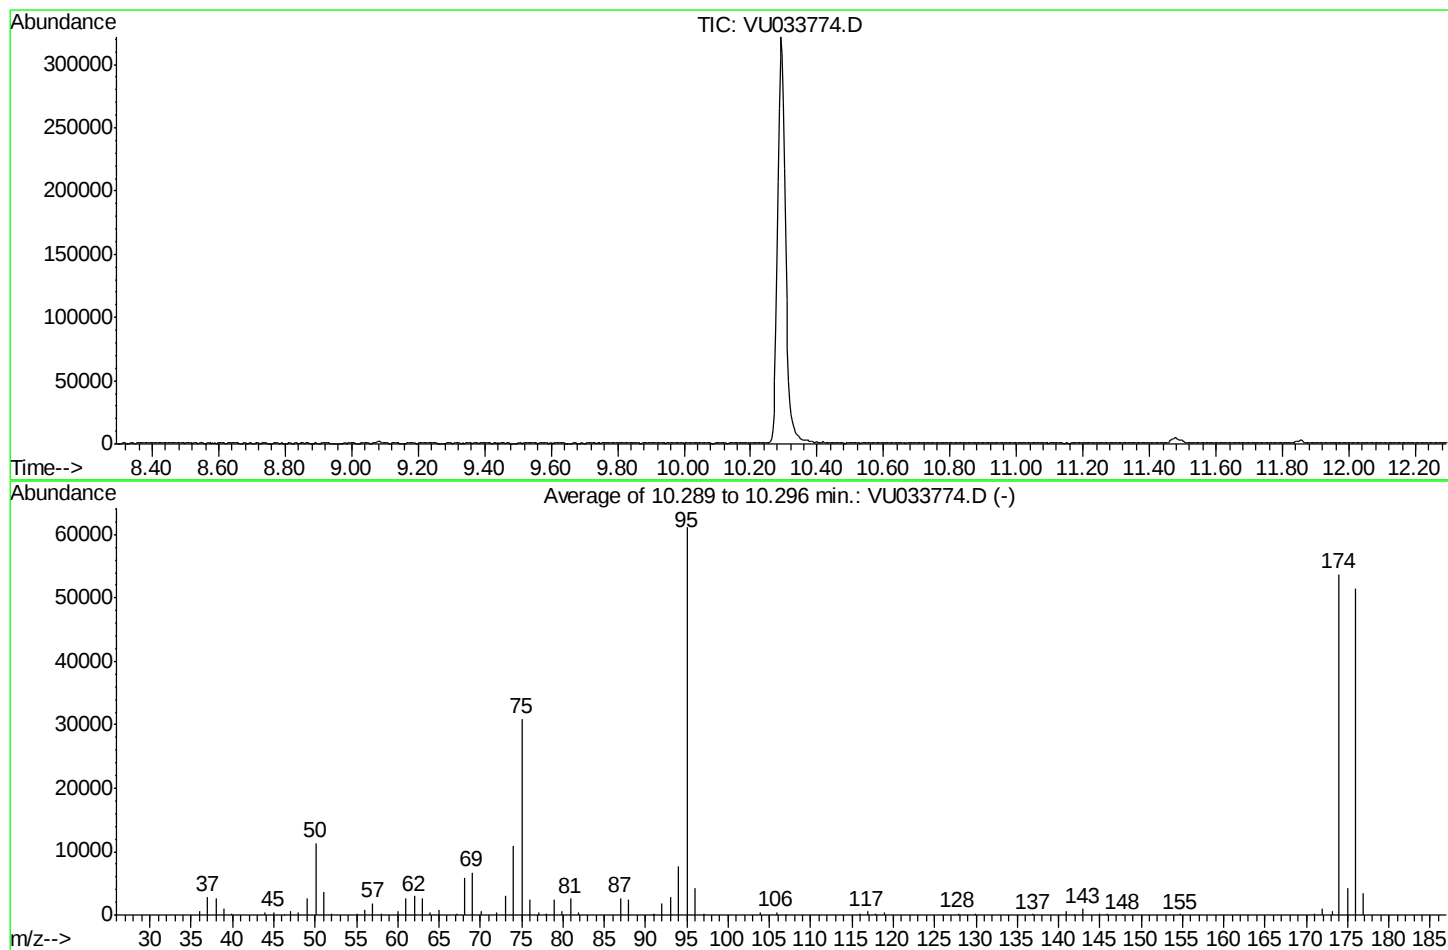

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11404	PASS
75	95	30	80	50.5	30906	PASS
95	95	100	100	100.0	61149	PASS
96	95	5	9	7.0	4258	PASS
173	174	0.00	2	1.3	708	PASS
174	95	50	120	88.0	53794	PASS
175	174	5	9	8.0	4319	PASS
176	174	95	101	95.8	51549	PASS
177	176	5	9	6.8	3528	PASS

m/z	Abundance
35.90	579.0
37.00	2717.0
38.00	2812.0
39.00	1151.0
39.90	324.0
43.90	780.0
45.00	493.0
46.20	141.0
47.10	690.0
47.90	439.0
49.00	2513.0
50.00	11137.0
51.00	3793.0
52.00	146.0
55.10	215.0
56.00	858.0
57.00	1893.0
57.90	103.0
60.00	728.0
61.00	2726.0
62.00	2998.0
63.00	2620.0
64.00	458.0
65.00	744.0
67.10	224.0
68.10	5613.0
69.00	6686.0
70.10	568.0
72.00	368.0
73.00	3207.0
74.00	10693.0
75.00	30728.0
76.00	2552.0
77.10	327.0
77.80	266.0
78.90	2382.0
79.90	720.0
80.90	2482.0
81.90	331.0
87.00	2445.0
88.00	2479.0
90.80	190.0
91.10	190.0
92.00	1845.0
93.00	2783.0
94.00	7451.0
95.00	60360.0
96.00	4149.0
97.10	121.0
103.90	307.0
105.90	363.0
107.00	105.0
116.00	187.0
116.90	489.0
117.90	258.0
118.90	475.0
128.00	210.0
129.80	211.0
136.90	107.0
140.80	593.0
141.90	122.0
143.00	948.0
145.00	309.0
146.00	102.0
147.80	102.0
154.80	194.0
171.00	169.0
171.90	890.0
174.00	51024.0
175.00	4479.0
176.00	49888.0
176.90	3470.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	549.0
37.00	2929.0
38.00	2739.0
39.00	1181.0
40.00	285.0
43.90	840.0
45.00	465.0
46.20	137.0
47.10	759.0
48.00	453.0
49.00	2686.0
50.10	11839.0
51.00	3763.0
52.00	141.0
55.10	184.0
56.00	818.0
57.00	1890.0
58.00	138.0
60.00	649.0
61.00	2733.0
62.00	3056.0
63.00	2621.0
64.00	451.0
65.00	764.0
67.10	230.0
68.00	5973.0
69.00	6920.0
70.10	545.0
72.00	349.0
73.00	3243.0
74.00	11236.0
75.00	31784.0
76.00	2590.0
77.10	382.0
78.10	318.0
78.90	2480.0
79.90	713.0
80.90	2659.0
81.90	435.0
87.00	2751.0
88.00	2397.0
91.10	209.0
92.00	1777.0
93.00	2900.0
94.00	7767.0
95.00	63000.0
96.00	4396.0
97.10	130.0
103.90	330.0
105.90	446.0
116.00	224.0
116.90	552.0
117.90	268.0
118.90	446.0
127.90	209.0
129.90	216.0
136.90	160.0
140.90	594.0
141.90	105.0
143.00	961.0
145.00	300.0
145.90	124.0
154.70	201.0
170.90	189.0
171.90	1004.0
173.10	1054.0
174.00	55528.0
175.00	4462.0
176.00	53488.0
177.00	3668.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	504.0
37.00	2916.0
38.00	2503.0
39.00	1123.0
40.00	230.0
44.00	854.0
44.90	384.0
47.00	672.0
48.00	431.0
49.00	2498.0
50.00	11237.0
51.00	3395.0
52.00	148.0
55.10	192.0
56.00	836.0
57.00	1725.0
58.00	172.0
60.10	505.0
61.00	2528.0
62.00	3013.0
63.00	2419.0
63.90	411.0
65.00	691.0
67.10	209.0
68.00	5860.0
69.00	6437.0
70.10	499.0
72.00	324.0
73.00	2846.0
74.00	10769.0
75.00	30208.0
76.00	2411.0
77.00	470.0
78.00	308.0
78.90	2372.0
79.90	614.0
80.90	2637.0
81.90	473.0
87.00	2748.0
88.00	2335.0
91.10	225.0
92.00	1679.0
93.00	2798.0
94.00	7520.0
95.00	60088.0
96.00	4231.0
97.00	133.0
103.90	302.0
105.90	440.0
116.00	254.0
116.90	529.0
117.80	276.0
118.90	391.0
127.80	214.0
129.80	207.0
136.90	160.0
140.90	578.0
143.00	907.0
145.00	276.0
145.90	127.0
147.80	124.0
154.70	169.0
170.90	194.0
171.90	1062.0
173.10	1071.0
174.00	54832.0
175.00	4018.0
176.00	51272.0
177.00	3447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Scan 2850 (10.254 min): VU033774.D
BFB55

m/z	Abundance
39.10	115.0
39.80	153.0
44.00	447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55