

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU081320\
 Data File : VU039847.D
 Acq On : 13 Aug 2020 13:42
 Operator : SY/MD
 Sample : L3647-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB7H8

Quant Time: Aug 14 02:07:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 14 01:47:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	76387	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	75215	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	36166	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	20257	4.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.20%
7) Chloroethane-d5	1.92	69	20460	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.58	63	28909	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.66	46	85673	47.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.44%
24) Chloroform-d	5.08	84	41889	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
26) 1,2-Dichloroethane-d4	5.72	65	27363	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
32) Benzene-d6	5.74	84	80044	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
36) 1,2-Dichloropropane-d6	6.70	67	28416	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.91	98	63200	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.60%
43) trans-1,3-Dichloropropene-	8.19	79	10760	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.64	63	58330	45.88	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.76%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	25650	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	29829	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
13) Acetone	2.66	43	4967	4.644 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU081320\
Data File : VU039847.D
Acq On : 13 Aug 2020 13:42
Operator : SY/MD
Sample : L3647-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB7H8

Quant Time: Aug 14 02:07:12 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 14 01:47:04 2020
Response via : Initial Calibration

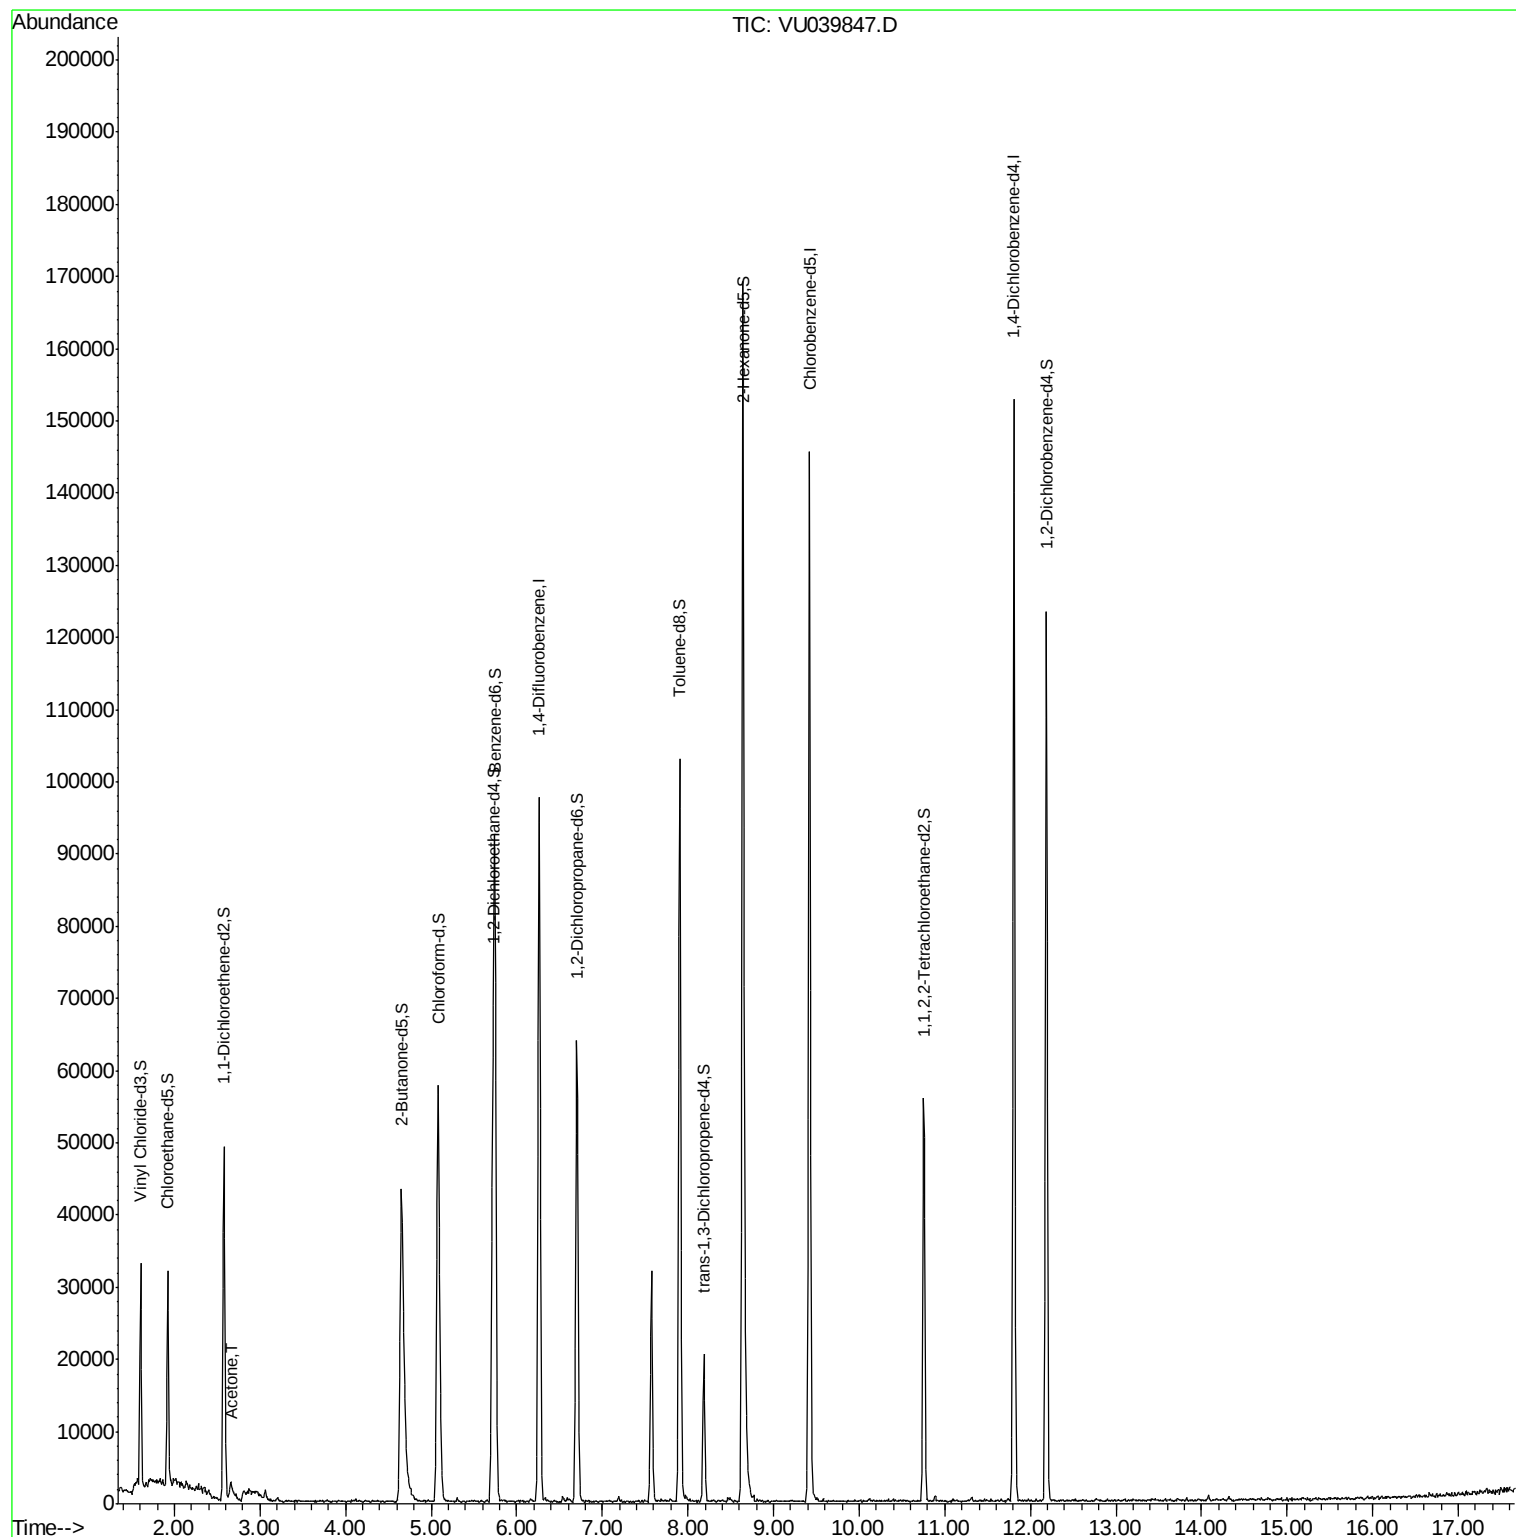

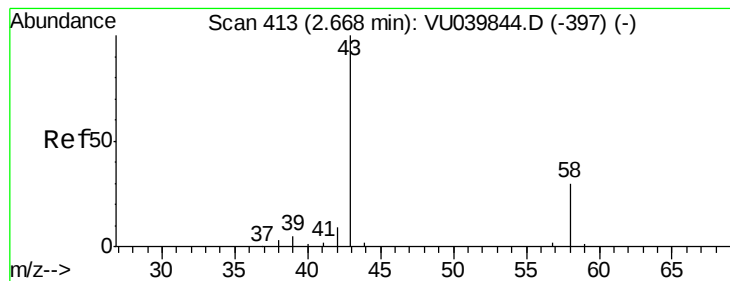

#13

Acetone

Concen: 4.644 ug/L

RT: 2.66 min Scan# 409

Delta R.T. -0.01 min

Lab File: VU039847.D

Acq: 13 Aug 2020 13:42

Instrument :
MSVOA_U
ClientSampleId :
CB7H8

Tot Ion: 43 Resp: 4967

Ion Ratio Lower Upper

43 100

58 26.2 0.0 61.8

