


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU081320\
 Data File : VU039843.D
 Acq On : 13 Aug 2020 09:16
 Operator : SY/MD
 Sample : BFB13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR080320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 14 01:47:04 2020

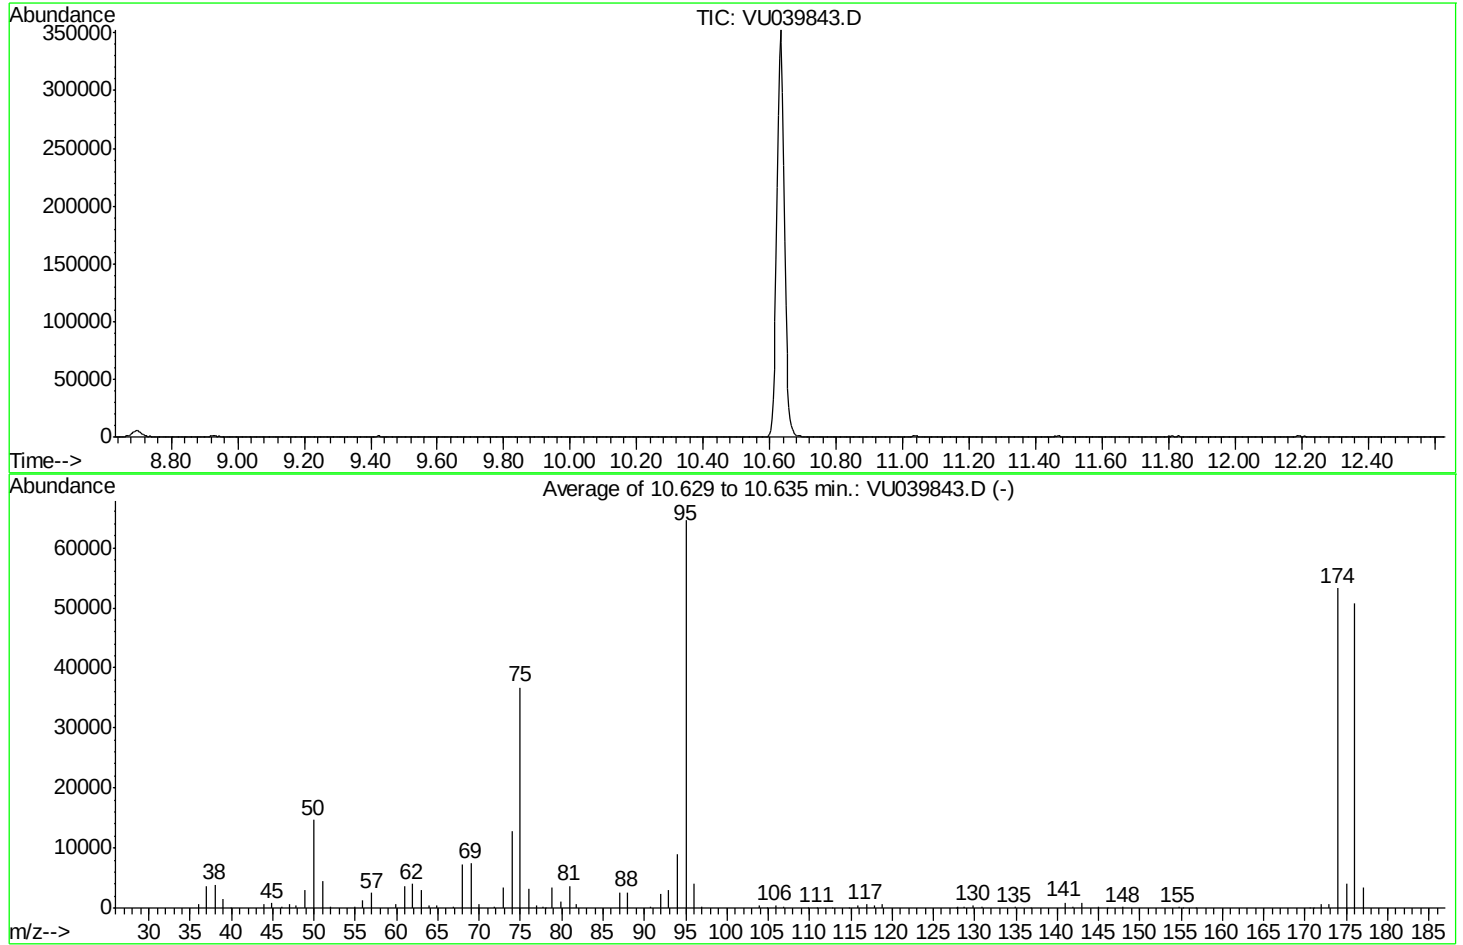

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	14646	PASS
75	95	30	80	56.9	36757	PASS
95	95	100	100	100.0	64570	PASS
96	95	5	9	6.2	3998	PASS
173	174	0.00	2	1.4	720	PASS
174	95	50	120	82.5	53293	PASS
175	174	5	9	7.5	4007	PASS
176	174	95	101	95.4	50845	PASS
177	176	5	9	6.5	3317	PASS

m/z	Abundance
36.00	524.0
36.90	3534.0
38.00	3974.0
39.00	1561.0
39.90	107.0
43.90	863.0
44.90	678.0
46.00	114.0
47.10	662.0
47.80	381.0
49.00	2881.0
49.90	14285.0
51.00	4391.0
52.00	187.0
54.90	273.0
55.90	1306.0
57.00	2432.0
60.00	555.0
60.90	3634.0
61.90	3872.0
63.00	3086.0
63.90	482.0
64.90	350.0
66.90	215.0
67.90	7354.0
69.00	7228.0
70.00	645.0
71.90	394.0
73.00	3266.0
74.00	12366.0
75.00	35336.0
76.00	3399.0
76.90	497.0
77.60	237.0
78.00	177.0
78.90	3369.0
79.90	1001.0
80.90	3548.0
81.80	671.0
86.90	2359.0
87.90	2592.0
90.80	273.0
91.90	2204.0
92.90	2844.0
94.00	8745.0
95.00	62480.0
96.00	4000.0
96.90	225.0
103.90	317.0
104.90	119.0
105.90	401.0
106.80	145.0
112.70	129.0
115.90	331.0
116.90	598.0
117.80	331.0
118.90	584.0
127.80	272.0
128.70	130.0
129.90	284.0
130.90	113.0
134.90	169.0
140.90	922.0
142.00	125.0
142.90	808.0
145.00	152.0
147.90	199.0
154.70	119.0
171.90	597.0
172.90	605.0
174.00	50352.0
175.00	4174.0
176.00	47648.0
177.00	3104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	582.0
36.90	3701.0
38.00	4036.0
39.00	1669.0
39.90	110.0
43.90	880.0
44.90	861.0
46.10	148.0
47.10	673.0
47.80	388.0
49.00	3092.0
49.90	15167.0
51.00	4593.0
51.90	138.0
55.00	268.0
55.90	1385.0
57.00	2600.0
59.90	607.0
61.00	3807.0
61.90	4176.0
63.00	3166.0
64.00	469.0
64.90	359.0
66.90	269.0
67.90	7477.0
69.00	7559.0
70.00	771.0
71.90	325.0
73.00	3450.0
74.00	13058.0
75.00	38136.0
76.00	3320.0
76.90	461.0
77.60	301.0
78.90	3546.0
79.90	1024.0
80.90	3786.0
81.80	719.0
87.00	2664.0
87.90	2714.0
90.70	270.0
91.90	2378.0
93.00	2974.0
94.00	9310.0
95.00	67024.0
96.00	4105.0
96.90	210.0
103.80	334.0
104.90	108.0
105.90	406.0
106.80	165.0
109.80	114.0
111.00	123.0
112.70	104.0
115.90	411.0
116.90	682.0
117.80	381.0
118.90	575.0
128.00	319.0
128.70	151.0
129.80	367.0
130.90	158.0
134.90	187.0
136.80	122.0
140.90	947.0
142.00	139.0
142.90	843.0
145.00	137.0
148.00	206.0
154.70	147.0
155.20	115.0
156.80	165.0
172.00	591.0
172.90	737.0
174.00	54960.0
175.00	4090.0
176.00	52560.0
177.00	3446.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
35.90	605.0
36.90	3431.0
38.00	3614.0
39.00	1532.0
43.90	892.0
44.90	847.0
46.10	149.0
47.00	691.0
47.80	398.0
48.90	2990.0
49.90	14488.0
51.00	4289.0
51.90	118.0
55.00	229.0
55.90	1298.0
57.00	2562.0
59.90	607.0
61.00	3550.0
61.90	3889.0
63.00	2957.0
64.00	355.0
64.90	342.0
66.90	246.0
67.90	6966.0
69.00	7539.0
70.00	739.0
71.90	252.0
72.90	3341.0
74.00	12737.0
75.00	36800.0
76.00	2884.0
76.90	382.0
77.70	292.0
78.80	3382.0
79.90	900.0
80.90	3631.0
81.80	704.0
87.00	2481.0
87.90	2576.0
90.70	278.0
91.90	2318.0
93.00	3040.0
94.00	9024.0
95.00	64208.0
96.00	3890.0
96.90	189.0
103.80	358.0
105.90	390.0
106.80	158.0
109.70	141.0
110.90	169.0
114.80	128.0
115.90	419.0
116.90	628.0
117.80	395.0
118.80	475.0
128.00	348.0
128.70	119.0
129.90	387.0
130.90	167.0
134.70	187.0
136.80	170.0
140.90	867.0
141.90	137.0
142.90	965.0
145.00	112.0
146.00	114.0
148.00	185.0
154.70	130.0
155.20	117.0
156.80	172.0
170.50	120.0
171.10	106.0
172.00	558.0
172.90	818.0
174.00	54568.0
175.00	3758.0
176.00	52328.0
177.00	3403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2875 (10.584 min): VU039843.D
BFB13

m/z	Abundance
43.80	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13