
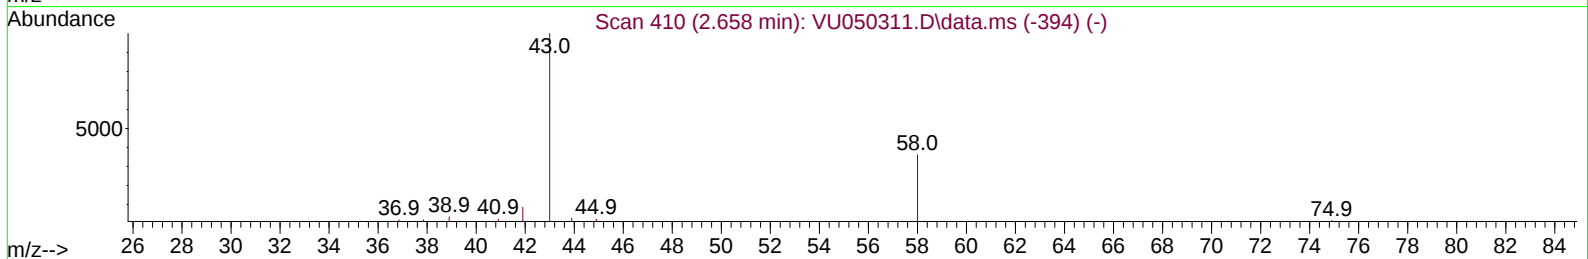
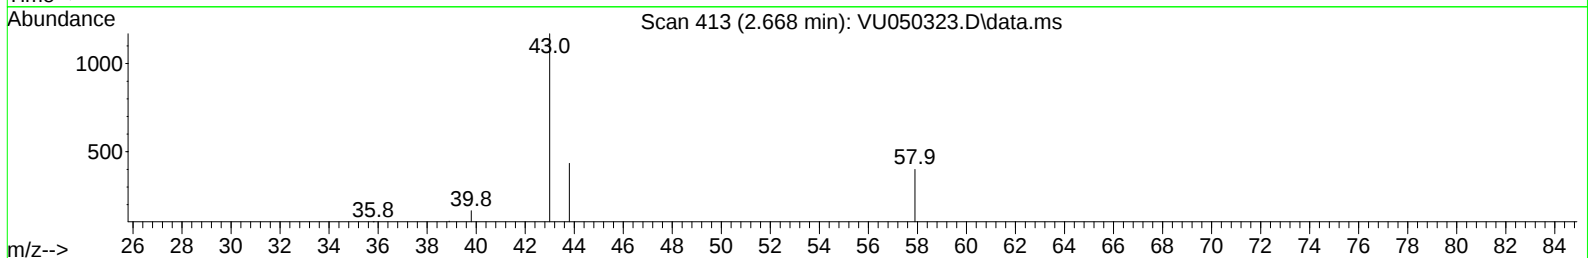


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050323.D
Acq On : 13 Aug 2022 17:04
Operator : SY/MD
Sample : N4072-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 14 01:28:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

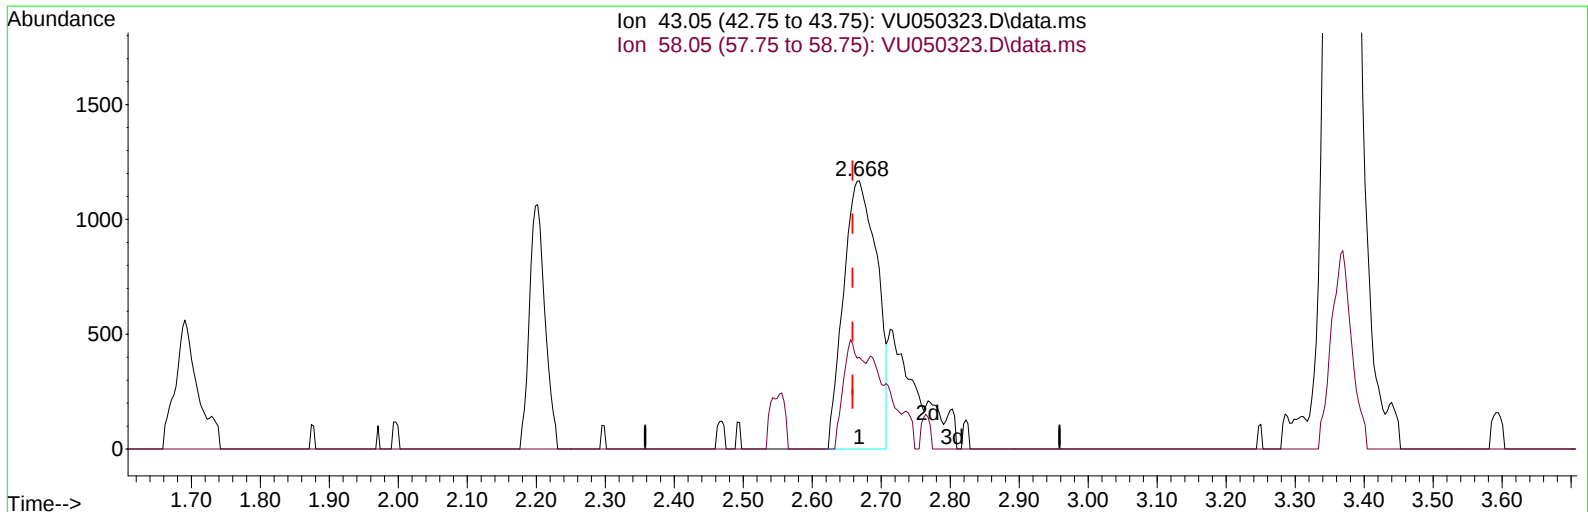

TIC: VU050323.D\data.ms

(13) Acetone (T)

2.668min (+ 0.010) 3.92 ug/L

response 3941

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.00	23.85
0.00	0.00	0.00
0.00	0.00	0.00