
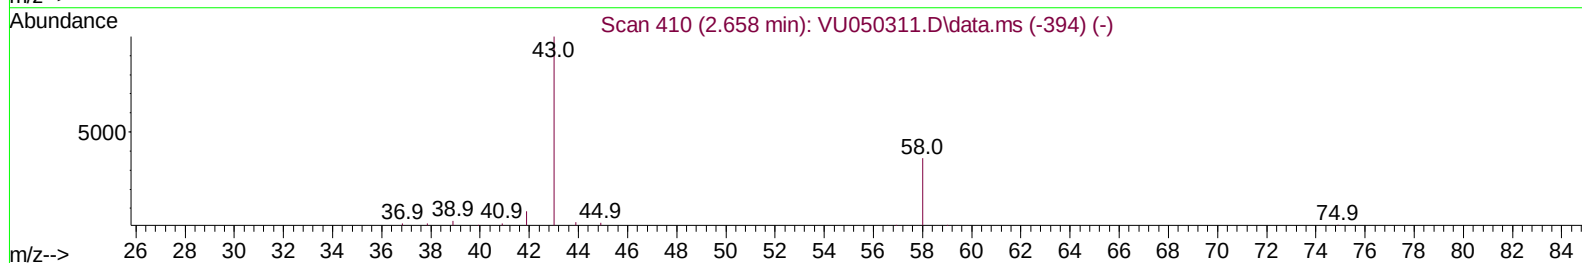
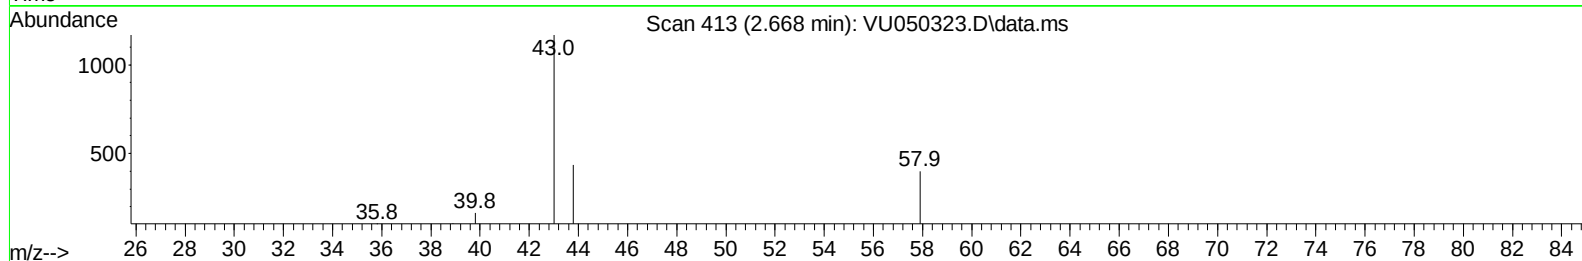


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050323.D
Acq On : 13 Aug 2022 17:04
Operator : SY/MD
Sample : N4072-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 14 01:28:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

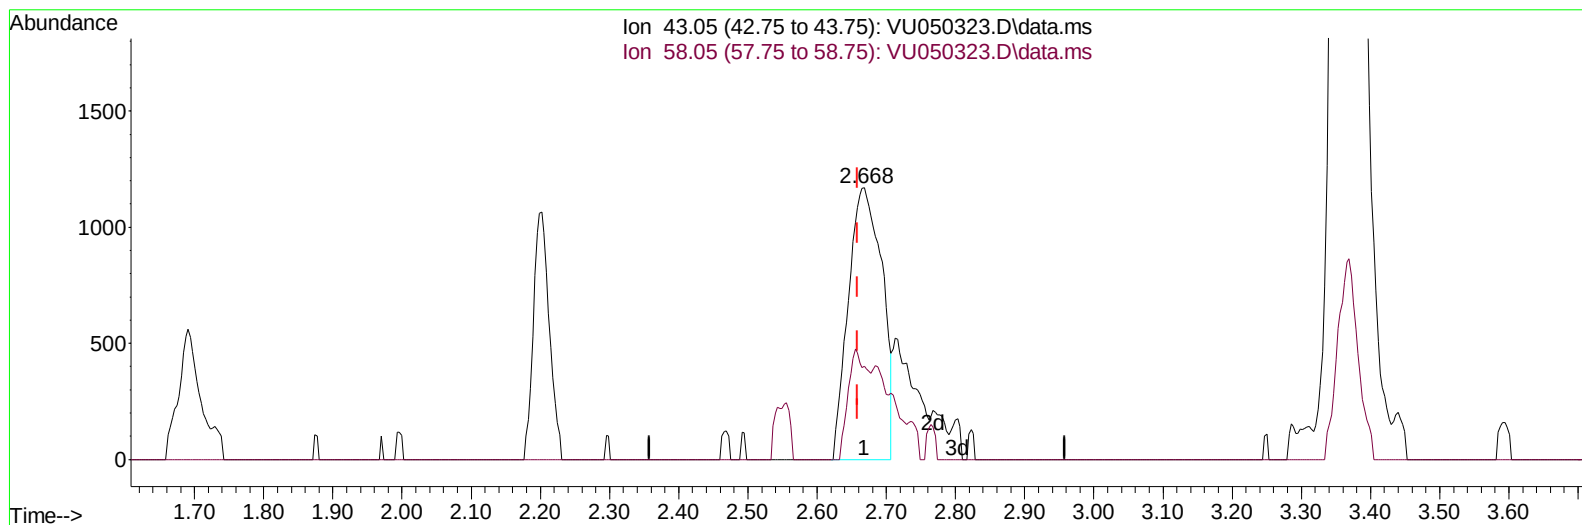




TIC: VU050323.D\data.ms

(13) Acetone (T)**2.668min (+ 0.010) 3.92 ug/L****response 3941**

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.00	23.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050323.D
Acq On : 13 Aug 2022 17:04
Operator : SY/MD
Sample : N4072-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 14 01:28:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

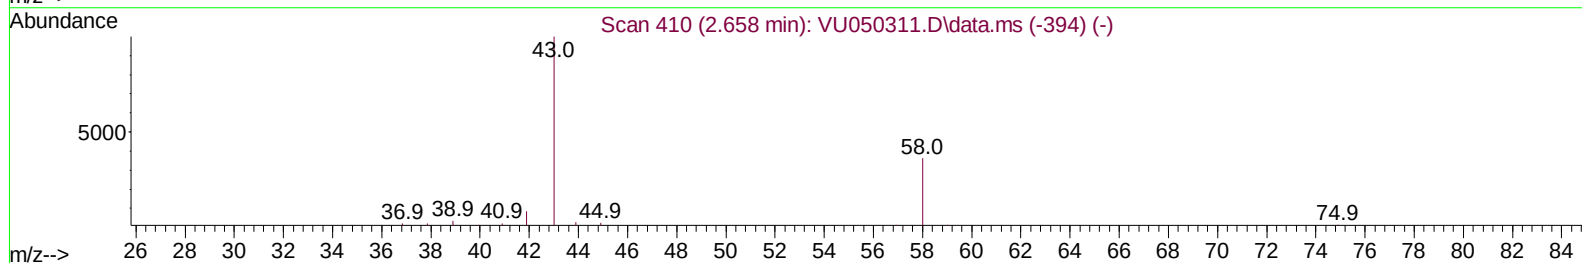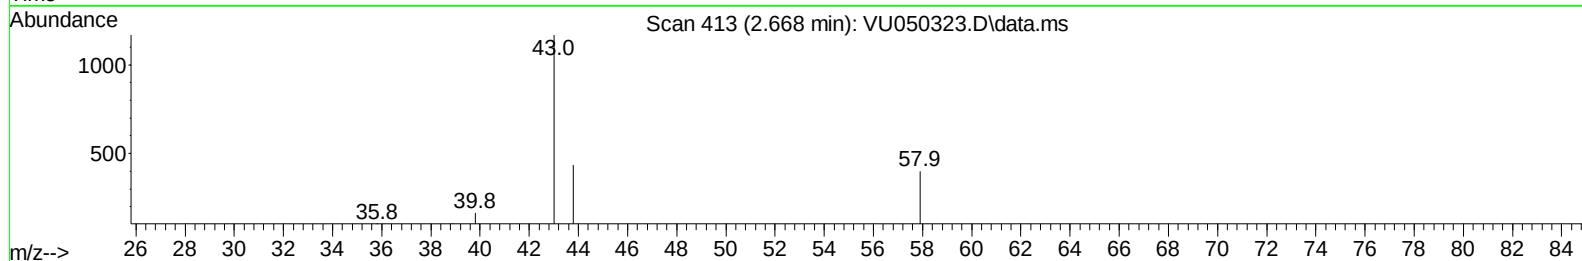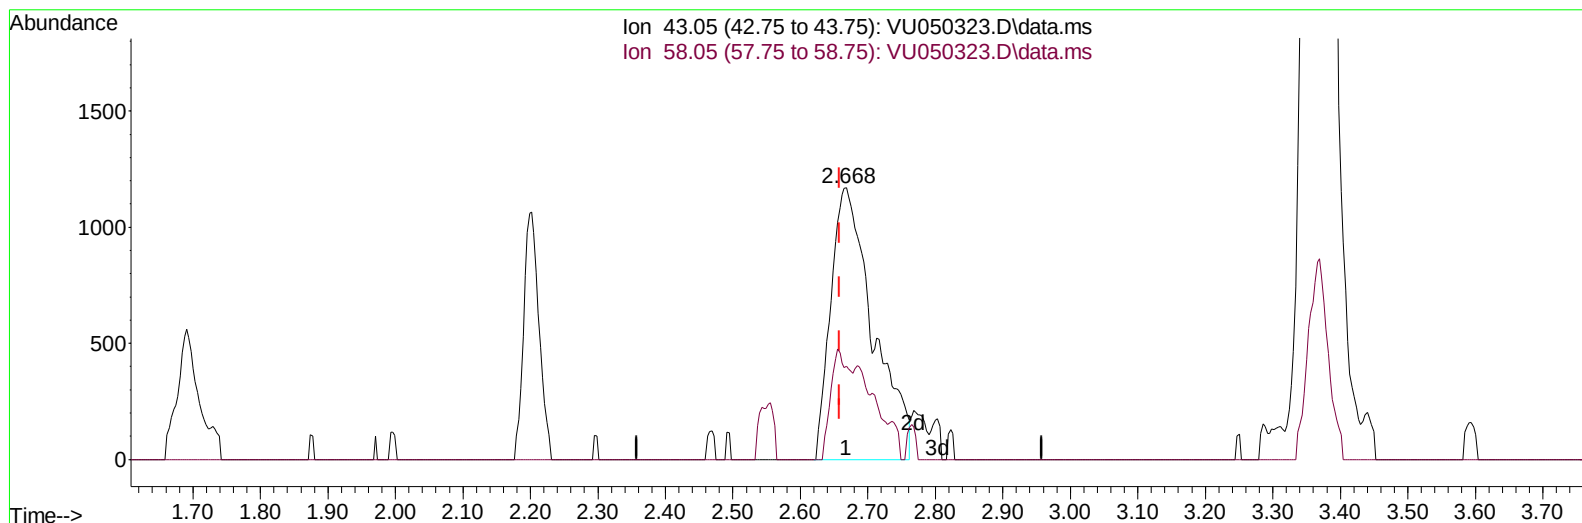

TIC: VU050323.D\data.ms

(13) Acetone (T)

2.668min (+ 0.010) 5.06 ug/L m

response 5087

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.00	18.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050323.D
 Acq On : 13 Aug 2022 17:04
 Operator : SY/MD
 Sample : N4072-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 14 01:28:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Aug 14 01:24:58 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	88999	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	89910	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	34819	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	42210	5.699	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 114.000%		
7) Chloroethane-d5	1.913	69	33916	5.676	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 113.600%		
11) 1,1-Dichloroethene-d2	2.562	65	16300	5.631	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 112.600%		
20) 2-Butanone-d5	4.649	46	115189	63.776	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 127.560%		
24) Chloroform-d	5.064	84	70788	5.138	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 102.800%		
26) 1,2-Dichloroethane-d4	5.703	65	37496	5.301	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 106.000%		
32) Benzene-d6	5.729	84	139756	4.981	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 99.600%		
36) 1,2-Dichloropropane-d6	6.690	67	48201	5.217	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 104.400%		
41) ToLuene-d8	7.899	98	108711	4.387	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 87.800%		
43) trans-1,3-Dichloroprop...	8.182	79	15737	4.753	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 95.000%		
46) 2-Hexanone-d5	8.636	63	64237	54.711	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 109.420%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	42539	5.243	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 104.800%		
66) 1,2-Dichlorobenzene-d4	12.192	152	38020	5.573	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 111.400%		
Target Compounds						
5) Vinyl chloride	1.601	62	4598	0.481	ug/L	# 82
13) Acetone	2.668	43	5087m	5.057	ug/L	
14) Carbon disulfide	2.790	76	6665	0.303	ug/L	99
17) Methyl tert-butyl Ether	3.369	73	114428	7.127	ug/L	98
18) trans-1,2-Dichloroethene	3.350	96	6436	0.934	ug/L	94
22) cis-1,2-Dichloroethene	4.665	96	14231	1.861	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050323.D
Acq On : 13 Aug 2022 17:04
Operator : SY/MD
Sample : N4072-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 14 01:28:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

