

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050315.D
 Acq On : 13 Aug 2022 13:47
 Operator : SY/MD
 Sample : N4115-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5E60

Quant Time: Aug 14 01:26:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Aug 14 01:24:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	93789	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	93833	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	40628	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43443	5.566	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.400%
7) Chloroethane-d5	1.912	69	35030	5.563	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.200%
11) 1,1-Dichloroethene-d2	2.565	65	16727	5.483	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	109.600%
20) 2-Butanone-d5	4.629	46	93910	49.339	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.680%
24) Chloroform-d	5.063	84	72891	5.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.703	65	37878	5.082	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.729	84	146416	5.000	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
36) 1,2-Dichloropropane-d6	6.690	67	49272	5.110	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.899	98	118221	4.571	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	8.179	79	15823	4.579	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.600%
46) 2-Hexanone-d5	8.636	63	51553	42.072	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.140%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	39239	4.634	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	40703	5.113	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%
Target Compounds						
16) Methylene chloride	3.044	84	12800	1.292	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050315.D
Acq On : 13 Aug 2022 13:47
Operator : SY/MD
Sample : N4115-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E60

Quant Time: Aug 14 01:26:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

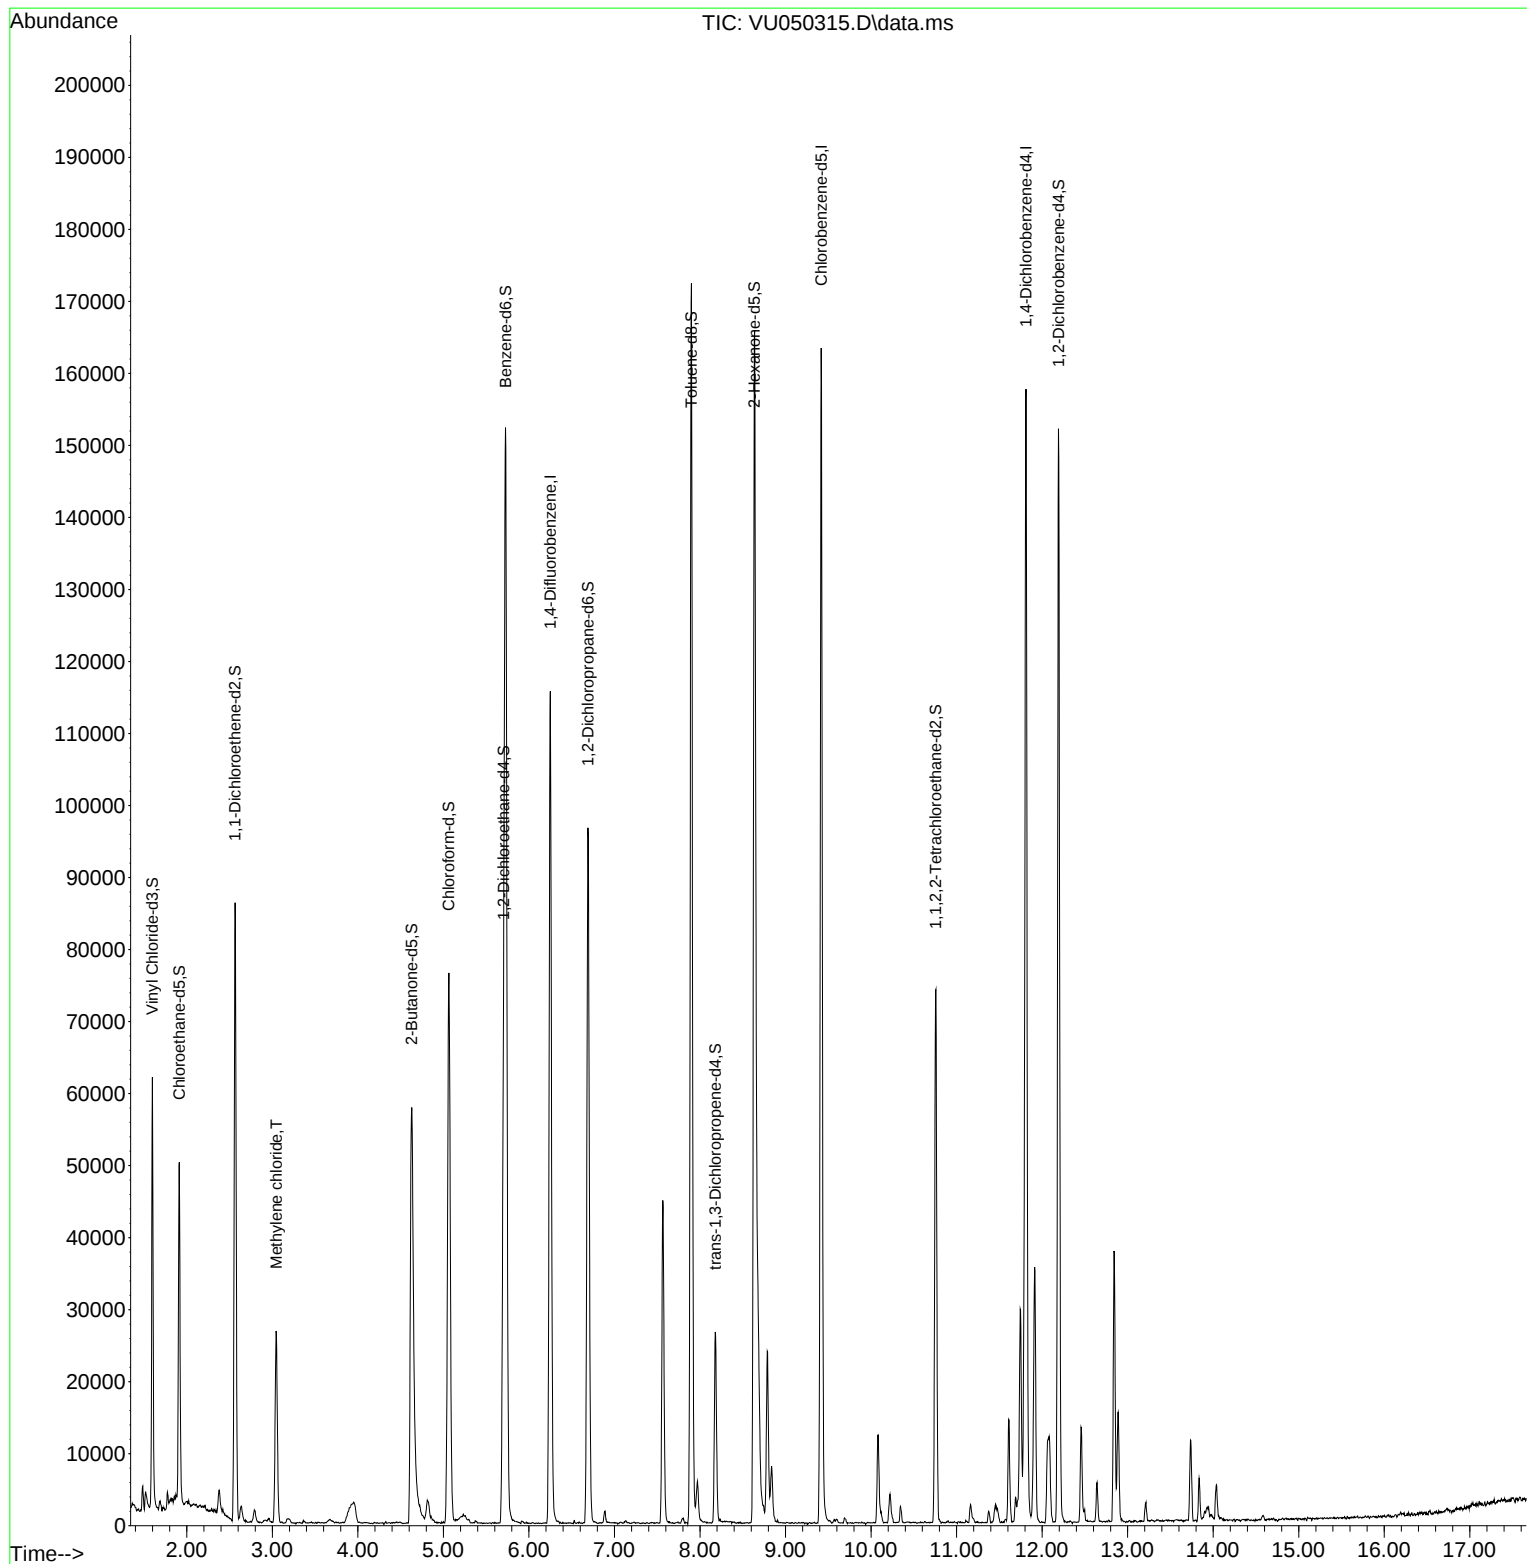

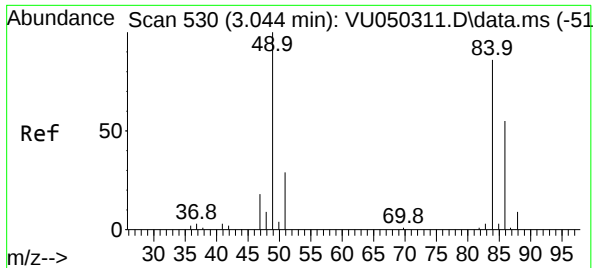

#16
Methylene chloride
Concen: 1.292 ug/L
RT: 3.044 min Scan# 51
Delta R.T. 0.000 min
Lab File: VU050315.D
Acq: 13 Aug 2022 13:47

Instrument :
MSVOA_U
ClientSampleId :
F5E60

Tgt Ion: 84 Resp: 12800
Ion Ratio Lower Upper
84 100
86 65.1 45.9 85.3
49 114.6 77.6 144.0

