

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050325.D
 Acq On : 13 Aug 2022 17:53
 Operator : SY/MD
 Sample : N4065-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Aug 14 01:28:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sun Aug 14 01:24:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	88789	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	90701	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	35261	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43067	5.829	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.600%
7) Chloroethane-d5	1.909	69	34811	5.839	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.800%
11) 1,1-Dichloroethene-d2	2.565	65	14981	5.188	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.800%
20) 2-Butanone-d5	4.626	46	103478	57.427	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.860%
24) Chloroform-d	5.063	84	72830	5.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.000%
26) 1,2-Dichloroethane-d4	5.700	65	38931	5.517	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.729	84	140055	4.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
36) 1,2-Dichloropropane-d6	6.690	67	47529	5.099	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.899	98	110836	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%
43) trans-1,3-Dichloroprop...	8.182	79	15580	4.665	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.200%
46) 2-Hexanone-d5	8.635	63	63656	53.743	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.480%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	41113	5.023	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	38056	5.508	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds						Qvalue
16) Methylene chloride	3.047	84	2297	0.245	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050325.D
Acq On : 13 Aug 2022 17:53
Operator : SY/MD
Sample : N4065-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Aug 14 01:28:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sun Aug 14 01:24:58 2022
Response via : Initial Calibration

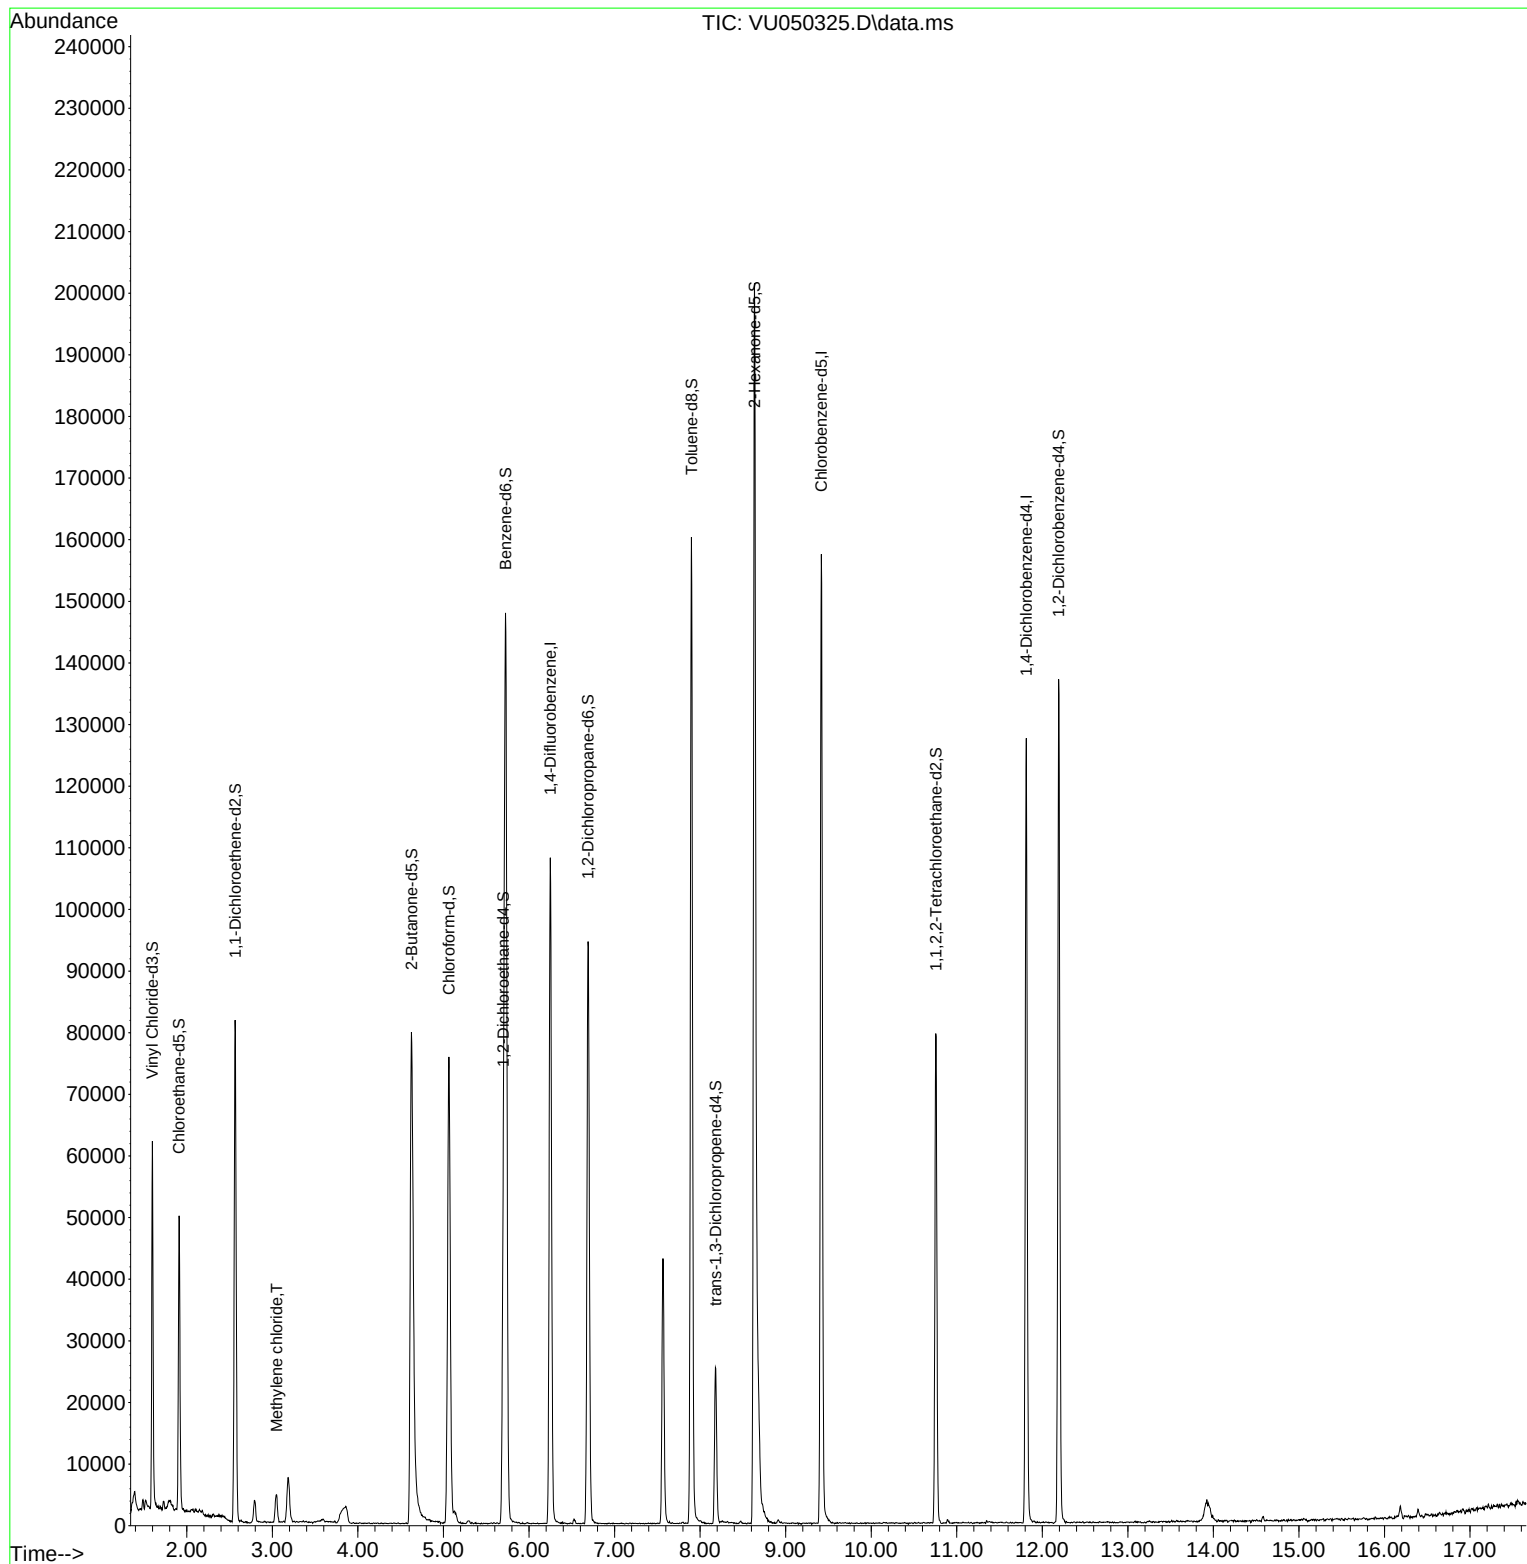

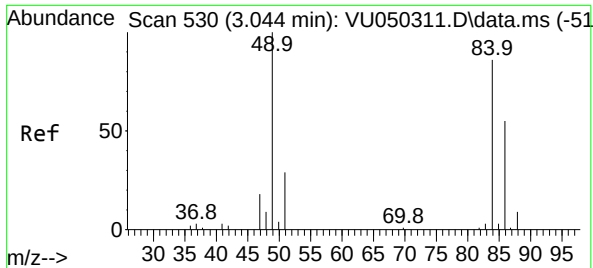

#16
Methylene chloride
Concen: 0.245 ug/L
RT: 3.047 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU050325.D
Acq: 13 Aug 2022 17:53

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

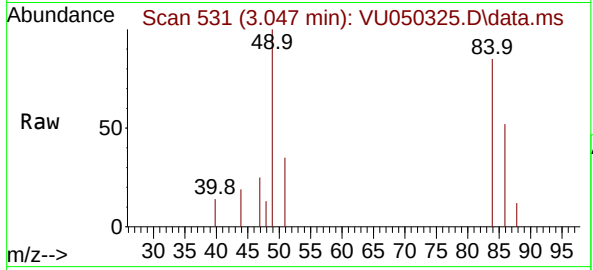

Tgt Ion: 84 Resp: 2297

Ion	Ratio	Lower	Upper
84	100		
86	61.0	45.9	85.3
49	118.0	77.6	144.0

