

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050312.D
 Acq On : 13 Aug 2022 12:27
 Operator : SY/MD
 Sample : VU0813WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK110

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.391	10	16	29	rVB3	2525	4342	1.03%	0.138%
2	1.597	72	80	94	rBV	59661	66129	15.61%	2.098%
3	1.729	116	121	131	rVB	3903	5034	1.19%	0.160%
4	1.912	169	178	191	rBV	48821	62313	14.71%	1.977%
5	2.565	369	381	397	rVB	87511	140471	33.17%	4.458%
6	3.044	517	530	543	rVB2	7276	12951	3.06%	0.411%
7	3.182	560	573	589	rVB	4913	10115	2.39%	0.321%
8	3.909	776	799	802	rBV	1971	5223	1.23%	0.166%
9	4.649	1011	1029	1071	rBV3	54483	213316	50.36%	6.769%
10	5.063	1143	1158	1178	rBV	77459	170291	40.21%	5.404%
11	5.726	1340	1364	1386	rBV2	157116	403847	95.35%	12.815%
12	6.250	1513	1527	1545	rBV	107000	201585	47.59%	6.397%
13	6.694	1648	1665	1688	rBV	98617	192212	45.38%	6.099%
14	7.568	1923	1937	1953	rBV	46321	81971	19.35%	2.601%
15	7.899	2028	2040	2058	rBV	173708	301057	71.08%	9.553%
16	8.182	2116	2128	2142	rBV	26801	45811	10.82%	1.454%
17	8.642	2257	2271	2309	rBV3	167970	423548	100.00%	13.441%
18	9.417	2500	2512	2540	rBV	151367	253307	59.81%	8.038%
19	10.758	2917	2929	2944	rBV	78099	126138	29.78%	4.003%
20	11.812	3246	3257	3279	rBV	124364	198250	46.81%	6.291%
21	12.195	3363	3376	3397	rBV	140013	233365	55.10%	7.405%




Sum of corrected areas: 3151276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050312.D
Acq On : 13 Aug 2022 12:27
Operator : SY/MD
Sample : VU0813WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

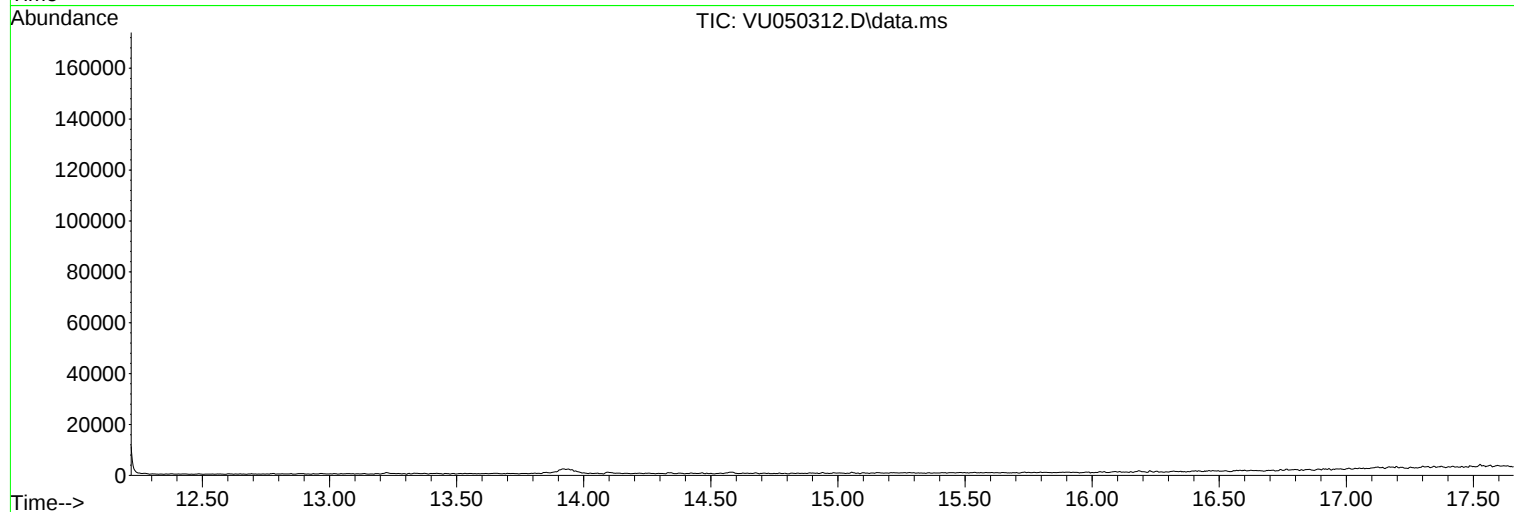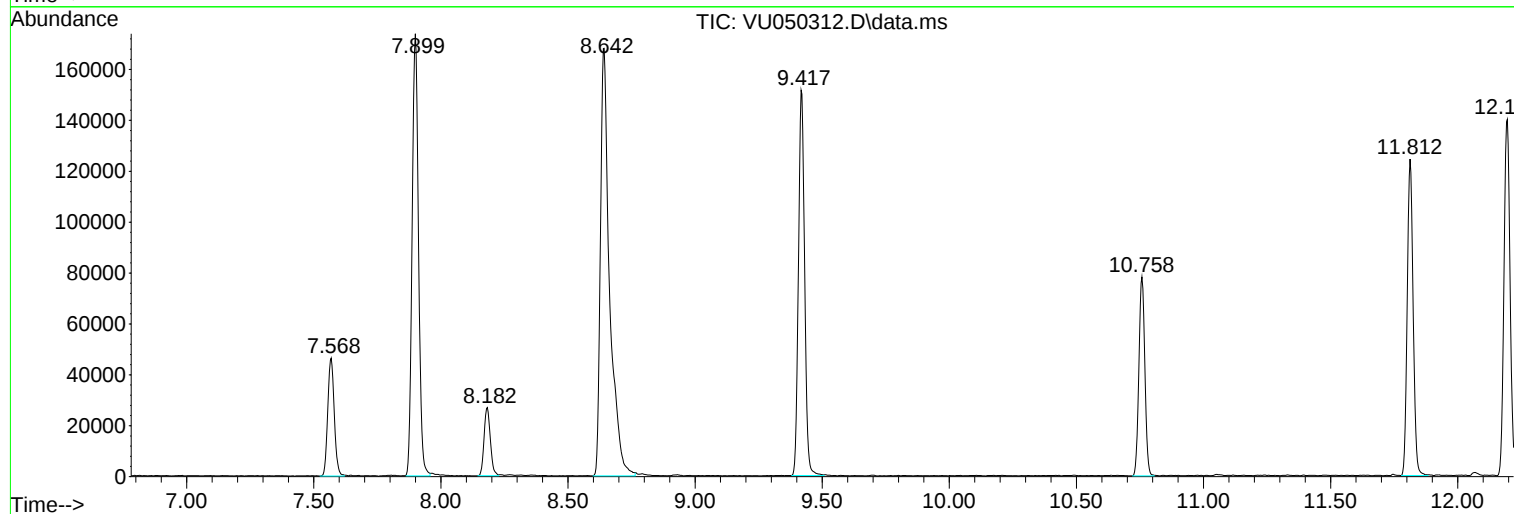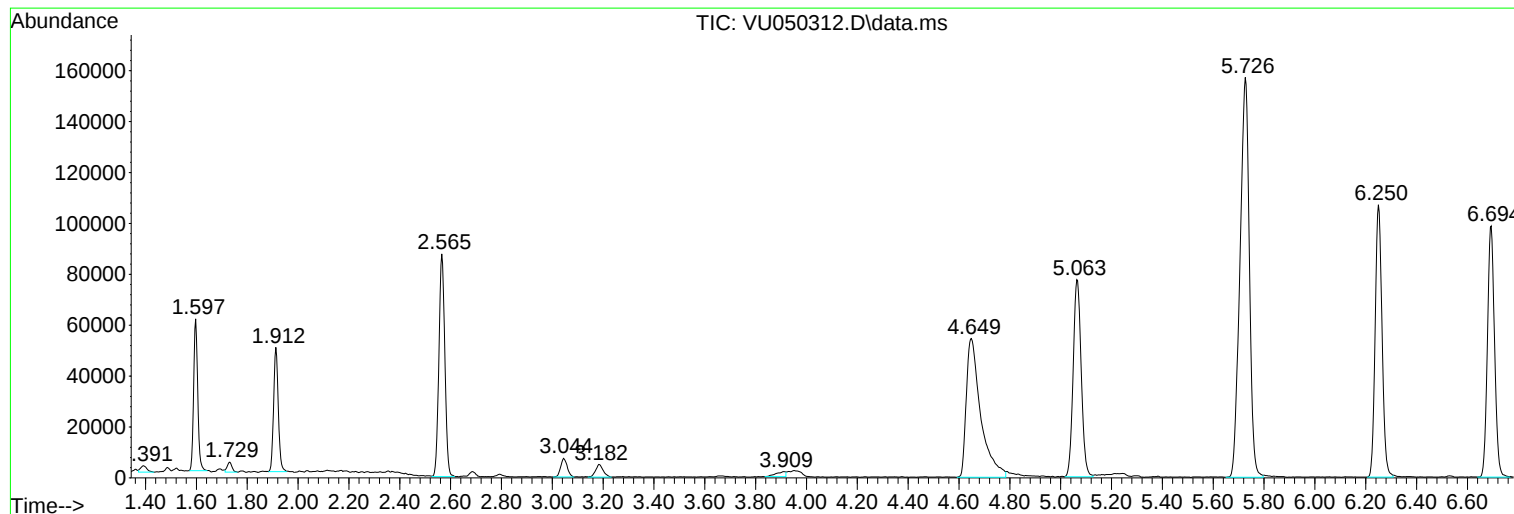

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050312.D
Acq On : 13 Aug 2022 12:27
Operator : SY/MD
Sample : VU0813WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050312.D
Acq On : 13 Aug 2022 12:27
Operator : SY/MD
Sample : VU0813WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK110

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc