

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050317.D
 Acq On : 13 Aug 2022 14:36
 Operator : SY/MD
 Sample : N4115-01DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5E00DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	99	rVB2	70278	84375	21.43%	2.729%
2	1.729	115	121	128	rBV	3978	4610	1.17%	0.149%
3	1.909	169	177	190	rVB	47316	61345	15.58%	1.984%
4	2.565	370	381	397	rBV	84964	136237	34.60%	4.406%
5	3.044	521	530	541	rBV2	5306	9603	2.44%	0.311%
6	3.186	560	574	589	rVB	8628	18574	4.72%	0.601%
7	3.838	753	777	779	rBV	2400	6187	1.57%	0.200%
8	4.626	1008	1022	1027	rBV2	74265	152773	38.80%	4.941%
9	5.063	1143	1158	1191	rBV	77062	174129	44.22%	5.632%
10	5.726	1344	1364	1387	rBV2	152954	393778	100.00%	12.736%
11	6.250	1511	1527	1548	rBV	115174	219183	55.66%	7.089%
12	6.542	1608	1618	1630	rVB3	13869	25223	6.41%	0.816%
13	6.690	1650	1664	1684	rBV	96507	186308	47.31%	6.026%
14	7.565	1922	1936	1952	rBV	44367	76961	19.54%	2.489%
15	7.899	2026	2040	2059	rBV	168779	294220	74.72%	9.516%
16	8.179	2117	2127	2142	rBV	26626	44434	11.28%	1.437%
17	8.636	2256	2269	2310	rBV3	165950	382943	97.25%	12.386%
18	9.417	2495	2512	2535	rBV	163100	272325	69.16%	8.808%
19	10.758	2916	2929	2945	rBV	74517	119631	30.38%	3.869%
20	11.812	3245	3257	3275	rBV	129131	207597	52.72%	6.714%
21	12.192	3363	3375	3395	rBV	135640	221373	56.22%	7.160%


Sum of corrected areas: 3091809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050317.D
Acq On : 13 Aug 2022 14:36
Operator : SY/MD
Sample : N4115-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

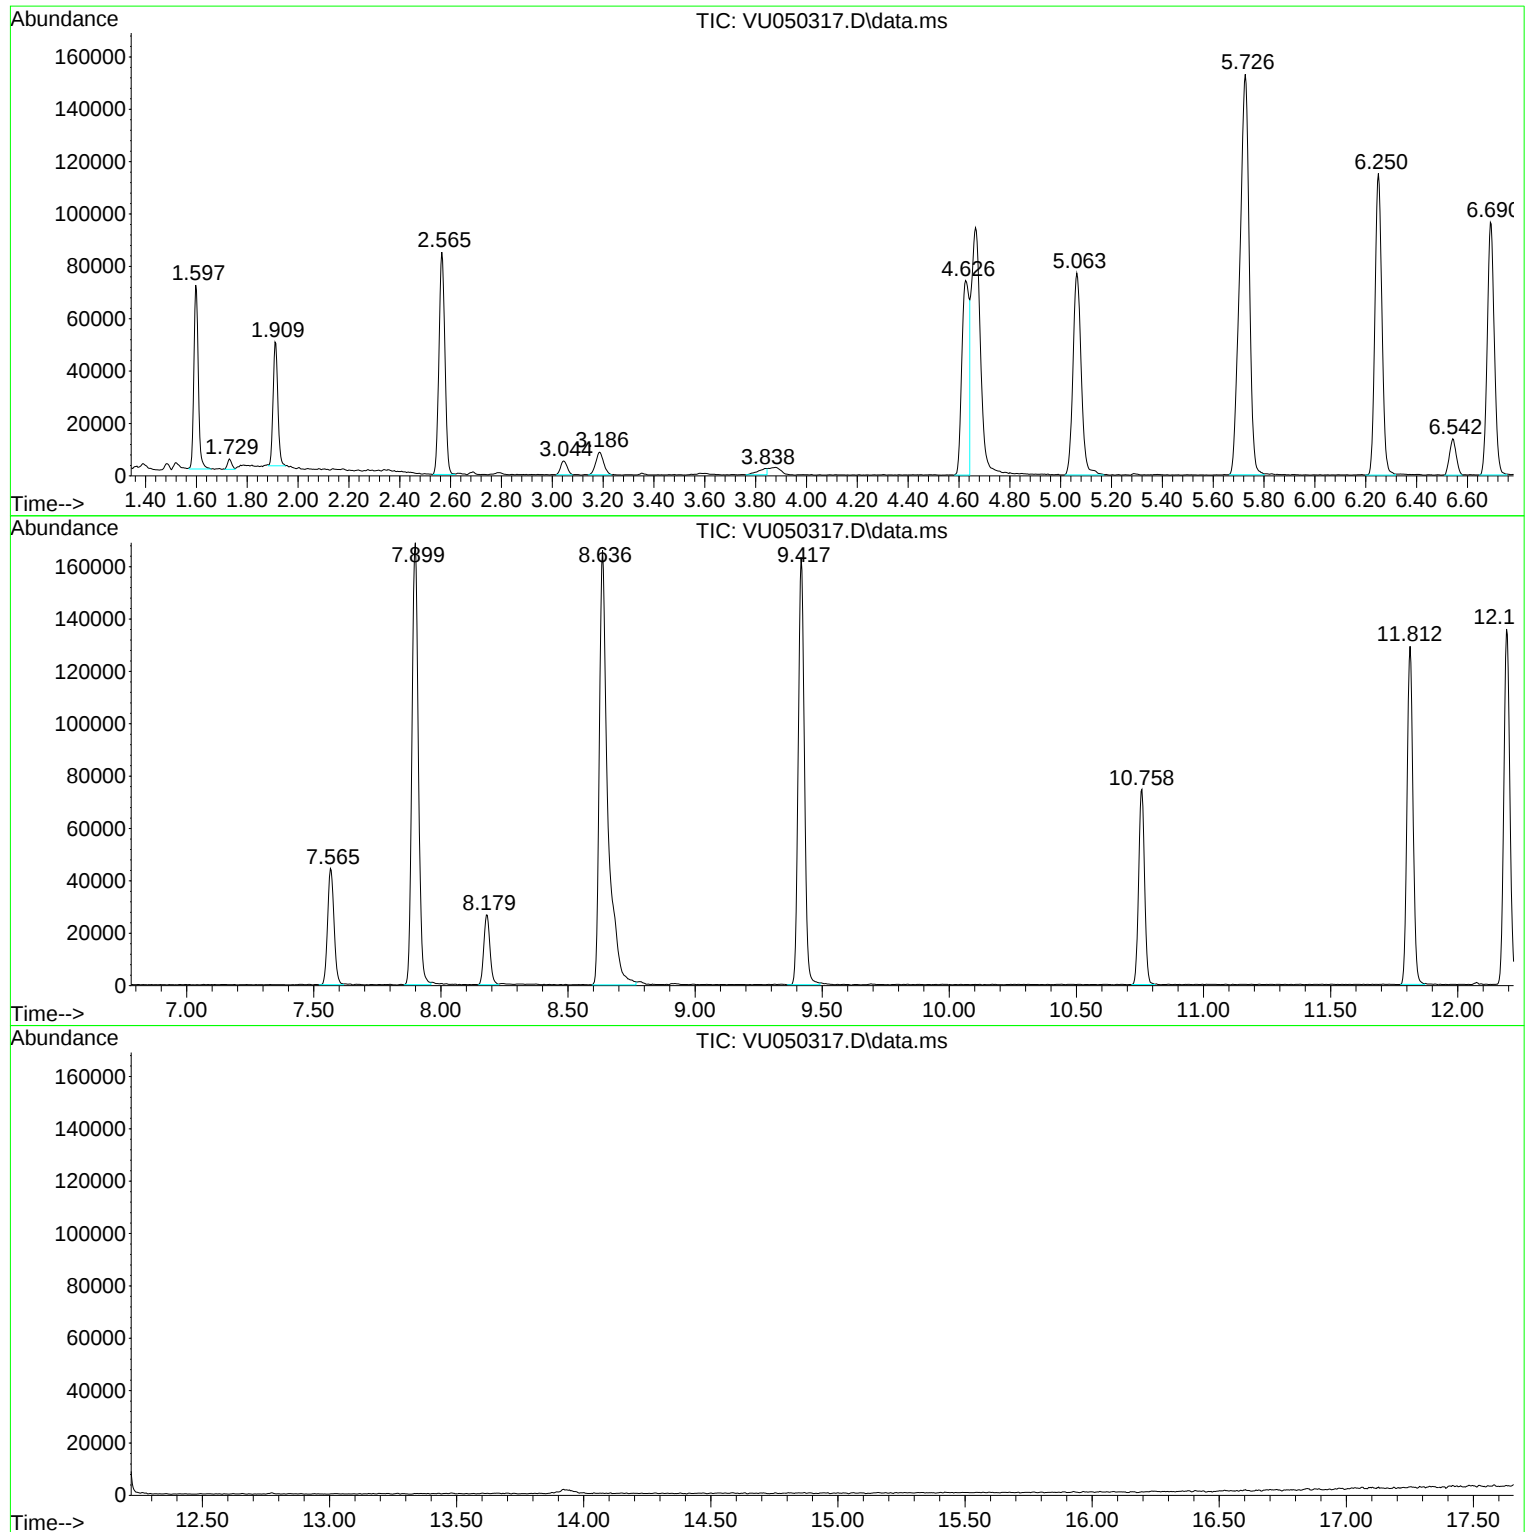

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050317.D
Acq On : 13 Aug 2022 14:36
Operator : SY/MD
Sample : N4115-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050317.D
Acq On : 13 Aug 2022 14:36
Operator : SY/MD
Sample : N4115-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc