

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050318.D
 Acq On : 13 Aug 2022 15:01
 Operator : SY/MD
 Sample : N4115-03DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5E44DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	71	81	103	rVB2	170573	209549	46.46%	6.157%
2	1.729	116	121	130	rVB	4214	5118	1.13%	0.150%
3	1.909	169	177	188	rBV	47750	60267	13.36%	1.771%
4	2.565	369	381	397	rVB	87205	140541	31.16%	4.129%
5	3.044	520	530	541	rVB2	6491	11224	2.49%	0.330%
6	3.186	559	574	593	rBV2	8294	18439	4.09%	0.542%
7	3.839	758	777	778	rBV	2453	5112	1.13%	0.150%
8	4.630	1009	1023	1055	rBV2	78624	253346	56.17%	7.444%
9	5.064	1143	1158	1193	rVB	78656	177690	39.40%	5.221%
10	5.726	1343	1364	1383	rBV2	156885	403690	89.51%	11.861%
11	6.250	1511	1527	1545	rBV	112623	211958	47.00%	6.228%
12	6.691	1649	1664	1690	rBV	99927	195828	43.42%	5.754%
13	7.568	1924	1937	1955	rBV	46421	81814	18.14%	2.404%
14	7.899	2026	2040	2060	rBV	172364	300294	66.58%	8.823%
15	8.179	2116	2127	2147	rBV	27632	45822	10.16%	1.346%
16	8.636	2257	2269	2306	rBV3	193031	451011	100.00%	13.252%
17	9.417	2499	2512	2532	rBV	159055	264972	58.75%	7.786%
18	10.755	2917	2928	2947	rVB	82450	131904	29.25%	3.876%
19	11.813	3246	3257	3273	rBV	127774	204002	45.23%	5.994%
20	12.192	3364	3375	3395	rBV	140408	230820	51.18%	6.782%


Sum of corrected areas: 3403401

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050318.D
Acq On : 13 Aug 2022 15:01
Operator : SY/MD
Sample : N4115-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

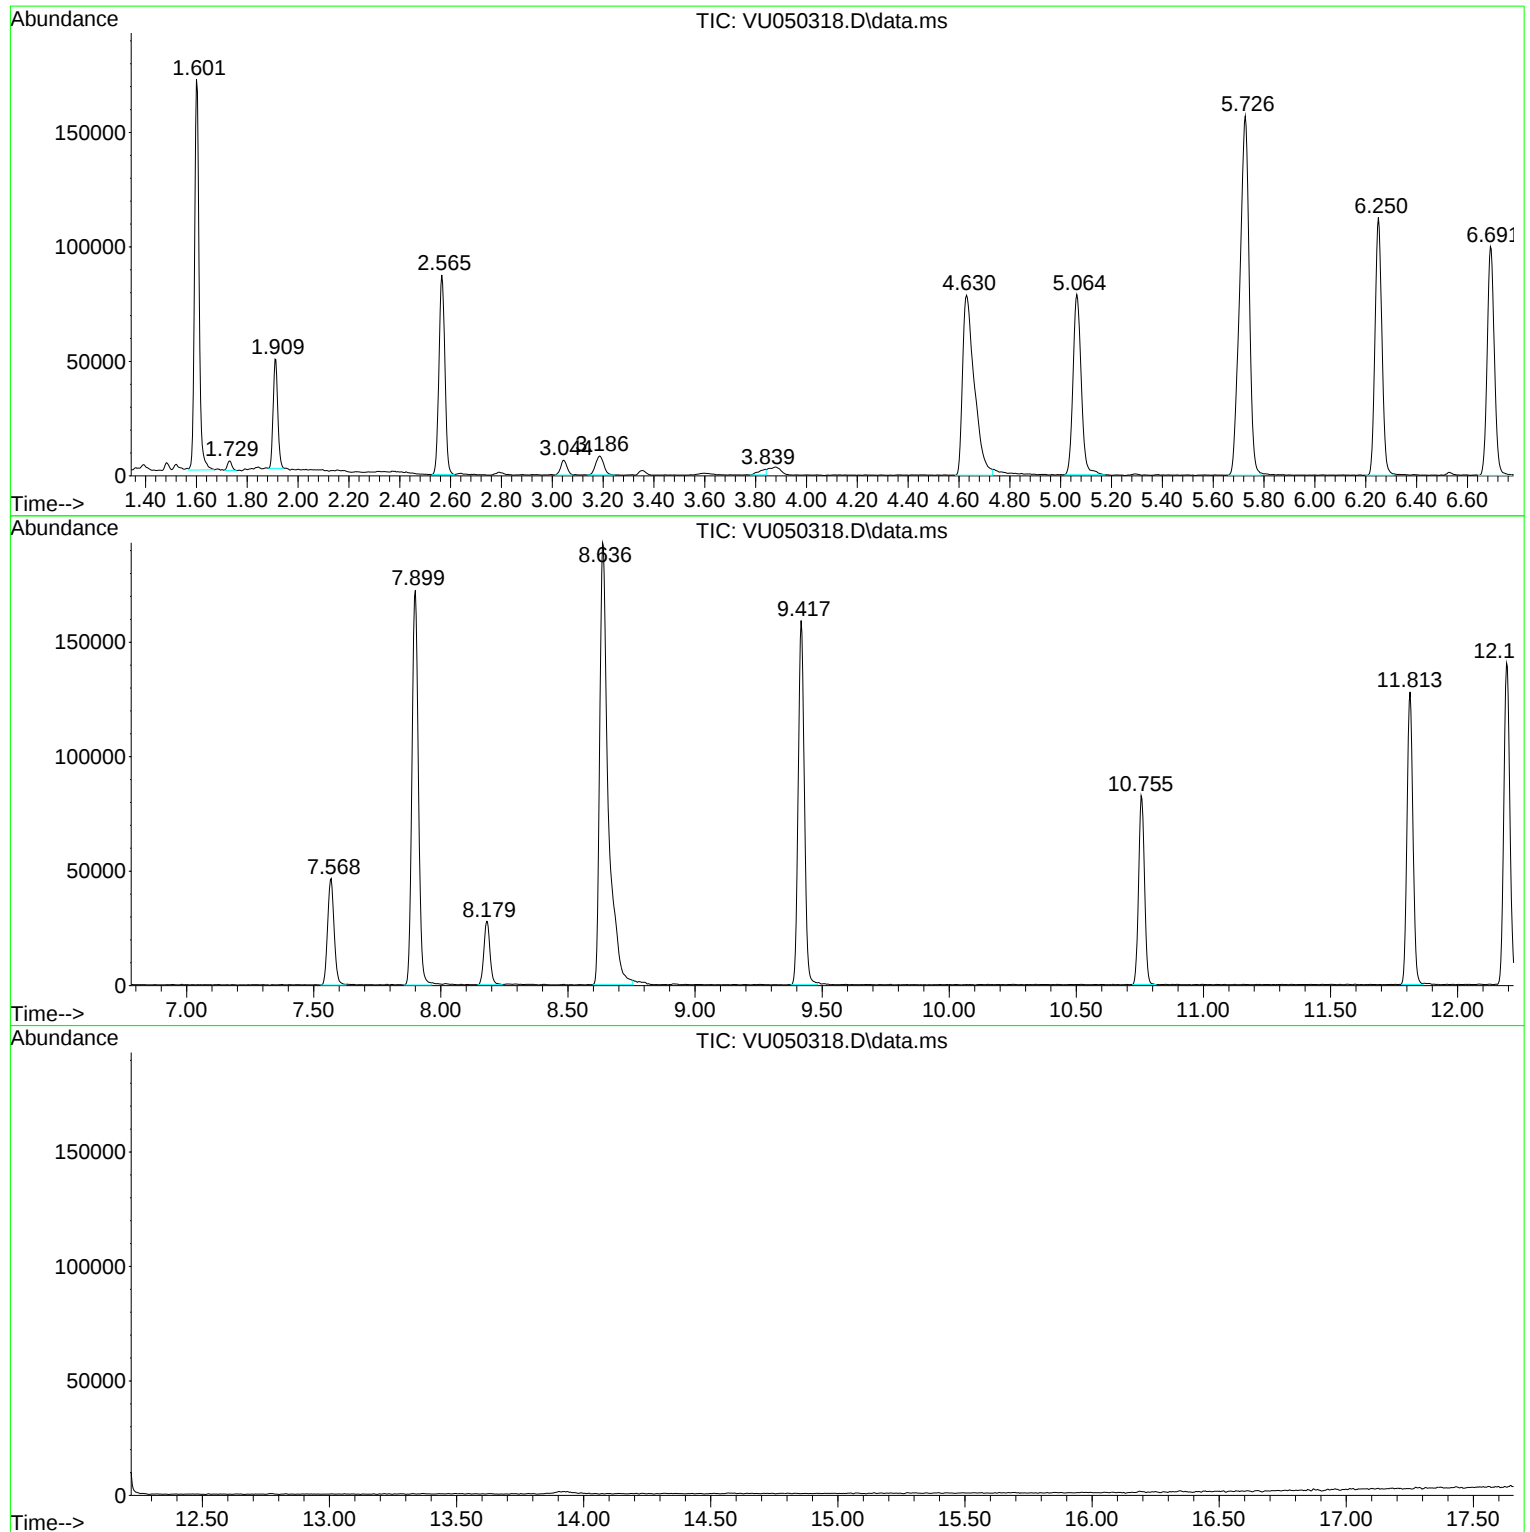

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050318.D
Acq On : 13 Aug 2022 15:01
Operator : SY/MD
Sample : N4115-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050318.D
Acq On : 13 Aug 2022 15:01
Operator : SY/MD
Sample : N4115-03DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc