

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050319.D
 Acq On : 13 Aug 2022 15:25
 Operator : SY/MD
 Sample : N4115-02DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5E01DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	70	rVV3	2834	4915	1.10%	0.155%
2	1.597	71	80	98	rVV2	81415	100897	22.54%	3.181%
3	1.909	169	177	194	rVB	49515	63693	14.23%	2.008%
4	2.565	370	381	395	rVB	86993	138863	31.02%	4.378%
5	3.044	521	530	545	rVB3	4061	7465	1.67%	0.235%
6	3.186	561	574	589	rBV2	7929	16994	3.80%	0.536%
7	3.896	773	795	797	rBV	2277	5505	1.23%	0.174%
8	4.636	1009	1025	1028	rBV2	81166	163565	36.54%	5.157%
9	5.063	1142	1158	1176	rBV	77660	171525	38.32%	5.408%
10	5.726	1343	1364	1391	rBV2	158732	405288	90.54%	12.778%
11	6.250	1511	1527	1550	rBV	109998	206049	46.03%	6.496%
12	6.539	1606	1617	1628	rBV7	4378	7729	1.73%	0.244%
13	6.690	1650	1664	1686	rVB	98337	192122	42.92%	6.057%
14	7.568	1925	1937	1953	rBV	45951	79644	17.79%	2.511%
15	7.899	2027	2040	2065	rBV	172699	299857	66.99%	9.454%
16	8.182	2116	2128	2141	rBV	27165	46308	10.35%	1.460%
17	8.635	2256	2269	2300	rBV2	188436	447629	100.00%	14.113%
18	9.417	2499	2512	2535	rBV	152637	255095	56.99%	8.043%
19	10.758	2916	2929	2948	rBV	82347	131156	29.30%	4.135%
20	11.812	3246	3257	3276	rBV	127115	198349	44.31%	6.254%
21	12.195	3363	3376	3398	rBV	140485	229069	51.17%	7.222%




Sum of corrected areas: 3171717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050319.D
Acq On : 13 Aug 2022 15:25
Operator : SY/MD
Sample : N4115-02DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

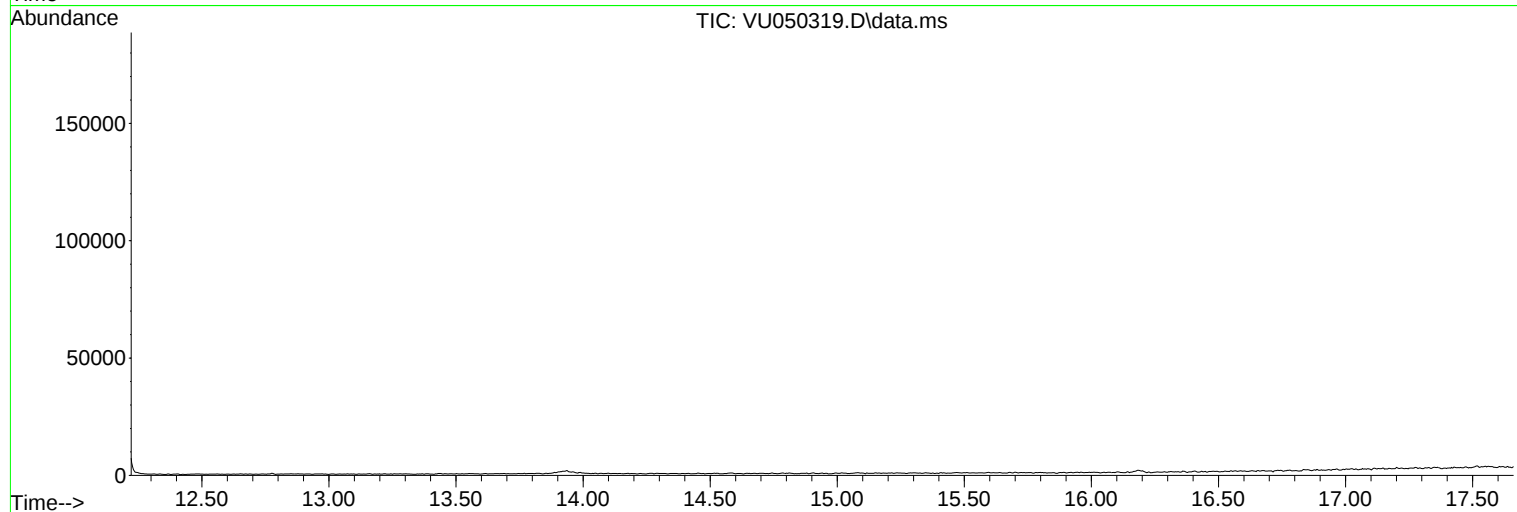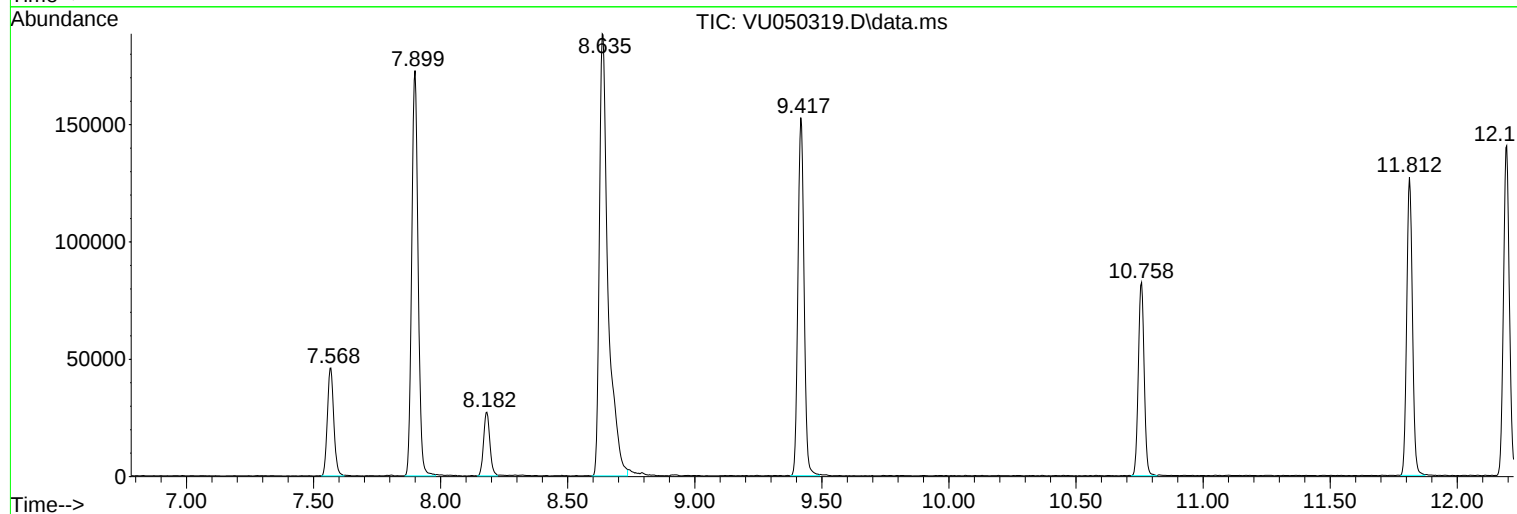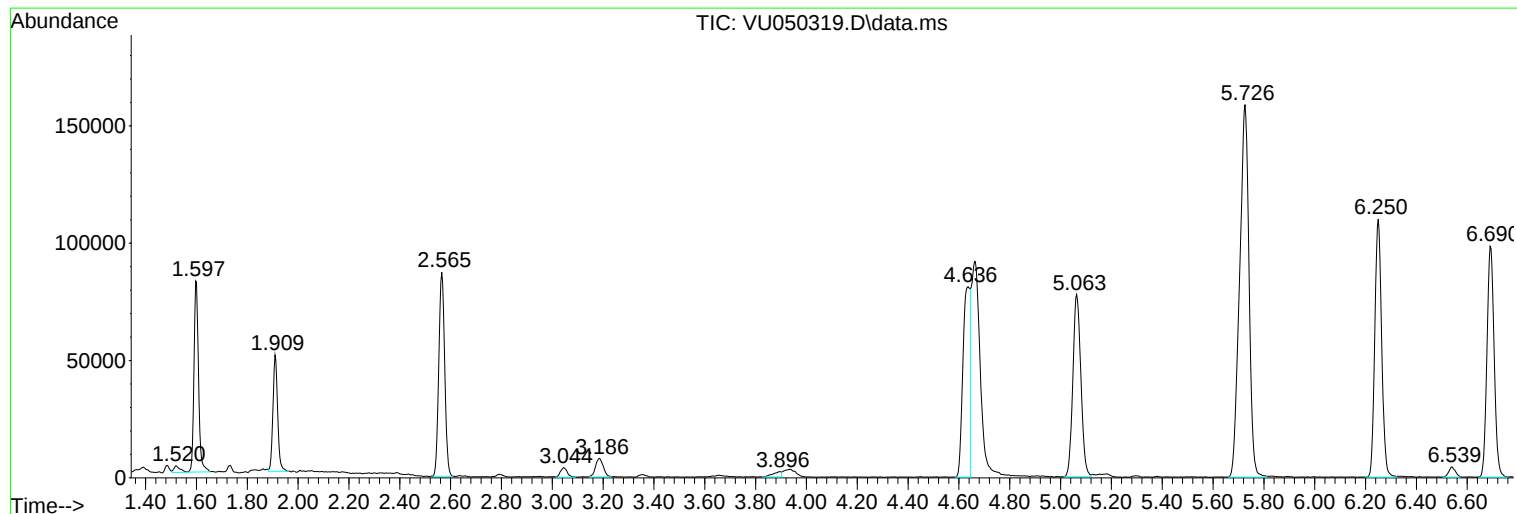

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050319.D
Acq On : 13 Aug 2022 15:25
Operator : SY/MD
Sample : N4115-02DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050319.D
Acq On : 13 Aug 2022 15:25
Operator : SY/MD
Sample : N4115-02DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5E01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc