

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050320.D
 Acq On : 13 Aug 2022 15:50
 Operator : SY/MD
 Sample : N4072-13DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUX0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	58073	65164	15.00%	1.944%
2	1.732	115	122	131	rVB	10166	12595	2.90%	0.376%
3	1.909	169	177	191	rVB	46715	60324	13.88%	1.800%
4	2.565	367	381	395	rBV	82765	131763	30.32%	3.931%
5	3.044	519	530	542	rBV2	5949	10885	2.51%	0.325%
6	3.186	559	574	594	rVB2	11081	25165	5.79%	0.751%
7	3.366	614	630	651	rBV2	85451	194790	44.83%	5.812%
8	4.629	1009	1023	1062	rBV2	79547	232792	53.57%	6.946%
9	5.063	1142	1158	1191	rVB	76279	171459	39.46%	5.116%
10	5.726	1344	1364	1383	rBV2	151864	387822	89.25%	11.572%
11	6.250	1514	1527	1548	rBV	112724	209722	48.26%	6.258%
12	6.690	1650	1664	1684	rBV	95593	185015	42.58%	5.520%
13	7.568	1925	1937	1953	rBV	43156	76369	17.58%	2.279%
14	7.899	2026	2040	2059	rBV	164214	286334	65.90%	8.543%
15	8.179	2116	2127	2144	rBV	26277	45067	10.37%	1.345%
16	8.639	2256	2270	2306	rBV3	184151	434525	100.00%	12.965%
17	9.417	2500	2512	2538	rBV	155080	263067	60.54%	7.849%
18	10.758	2917	2929	2945	rBV	79777	127955	29.45%	3.818%
19	11.812	3246	3257	3280	rBV	128295	205911	47.39%	6.144%
20	12.195	3364	3376	3400	rBV	137017	224766	51.73%	6.706%




Sum of corrected areas: 3351490

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050320.D
Acq On : 13 Aug 2022 15:50
Operator : SY/MD
Sample : N4072-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

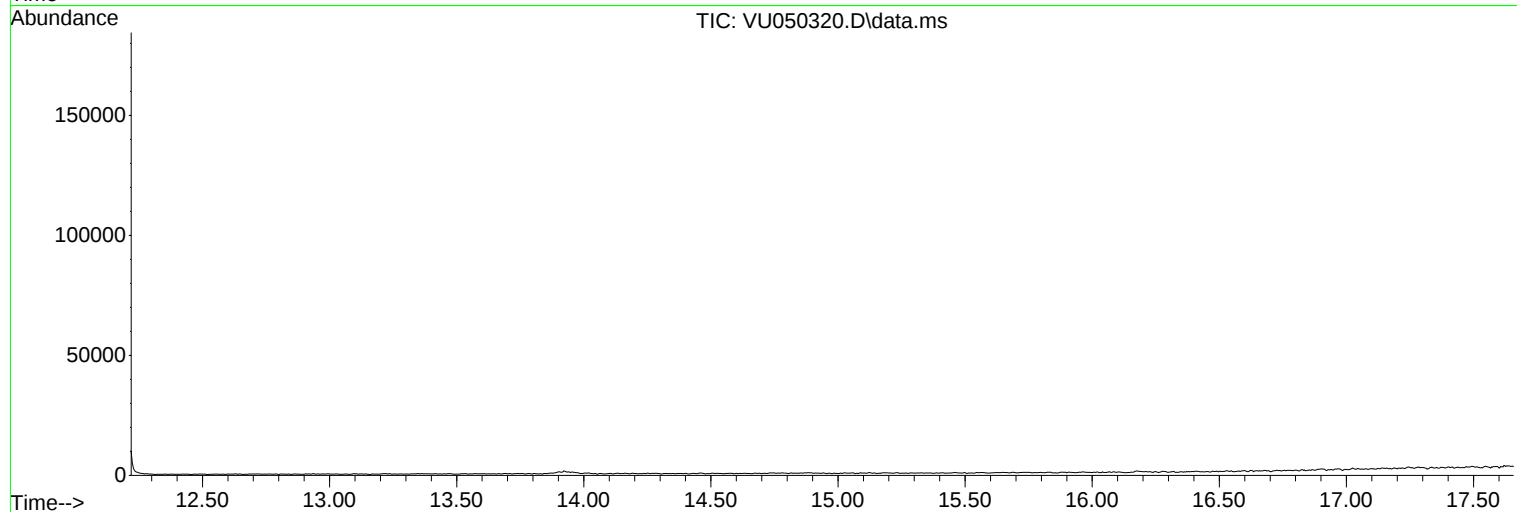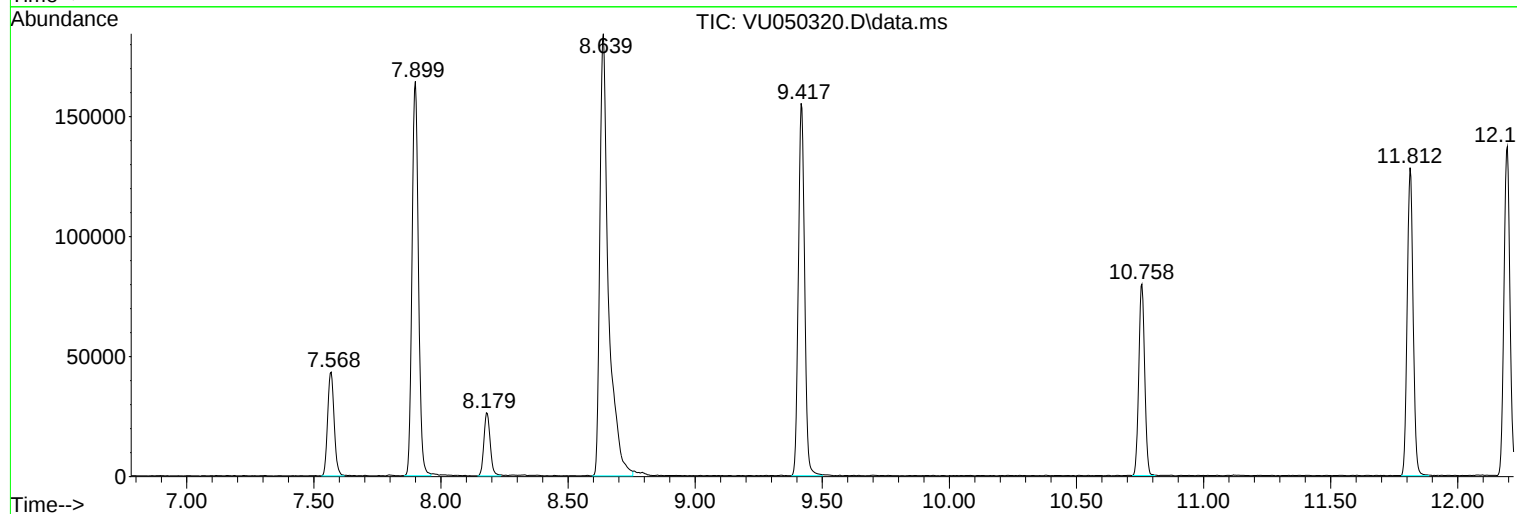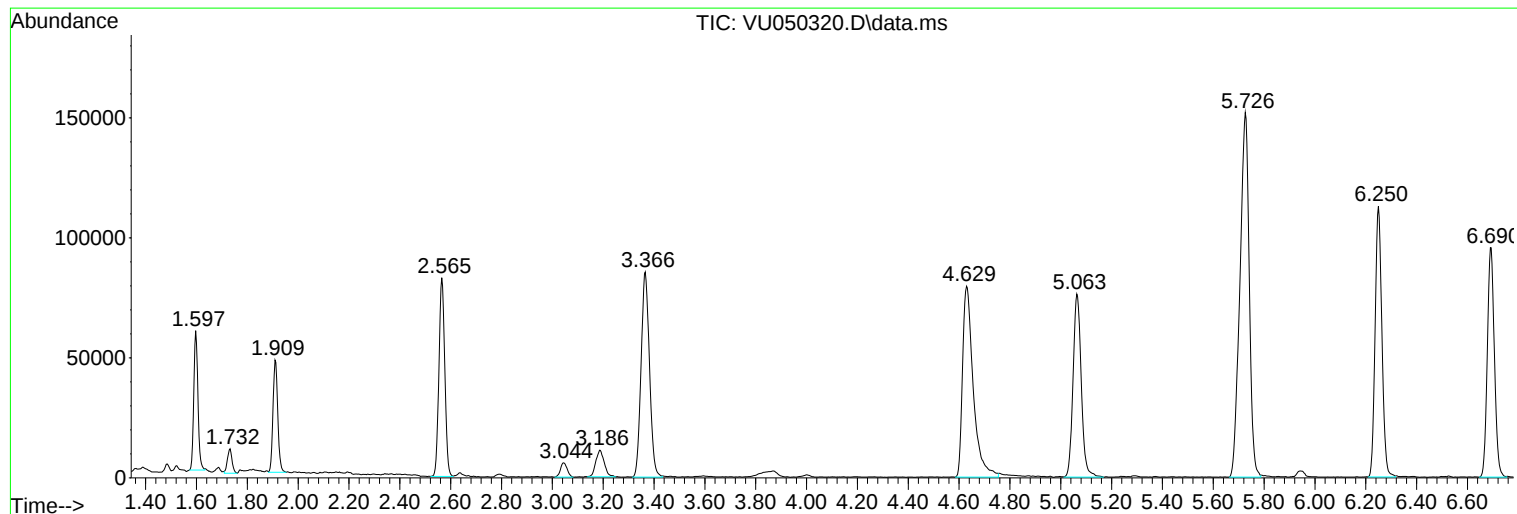

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050320.D
Acq On : 13 Aug 2022 15:50
Operator : SY/MD
Sample : N4072-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050320.D
Acq On : 13 Aug 2022 15:50
Operator : SY/MD
Sample : N4072-13DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUX0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc