

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050325.D
 Acq On : 13 Aug 2022 17:53
 Operator : SY/MD
 Sample : N4065-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.391	9	16	31	rVB3	3046	5895	1.37%	0.190%
2	1.597	72	80	91	rBV	59660	66987	15.58%	2.156%
3	1.909	169	177	190	rBV	47657	60739	14.12%	1.955%
4	2.565	370	381	395	rBV	81428	130667	30.39%	4.205%
5	2.793	439	452	461	rBV	3604	6400	1.49%	0.206%
6	3.047	521	531	540	rBV3	4430	8221	1.91%	0.265%
7	3.186	562	574	591	rBV2	7271	16379	3.81%	0.527%
8	3.858	750	783	804	rVB	2783	14218	3.31%	0.458%
9	4.626	1007	1022	1059	rBV2	79776	216357	50.31%	6.962%
10	5.063	1143	1158	1174	rBV	75612	167533	38.96%	5.391%
11	5.726	1343	1364	1383	rBV2	147729	381455	88.71%	12.275%
12	6.250	1514	1527	1548	rBV	108046	203543	47.33%	6.550%
13	6.690	1651	1664	1680	rBV	94471	183084	42.58%	5.892%
14	7.565	1921	1936	1957	rBV2	43044	75520	17.56%	2.430%
15	7.899	2027	2040	2069	rBV	160037	280268	65.18%	9.019%
16	8.179	2117	2127	2142	rBV	25306	43152	10.04%	1.389%
17	8.635	2257	2269	2303	rBV2	201236	430013	100.00%	13.838%
18	9.417	2500	2512	2531	rBV	157260	260514	60.58%	8.383%
19	10.754	2917	2928	2950	rVB	79515	126640	29.45%	4.075%
20	11.812	3244	3257	3280	rBV	127341	201562	46.87%	6.486%
21	12.192	3356	3375	3392	rBV	136987	223627	52.00%	7.196%
22	13.921	3902	3913	3917	rBV6	2519	4743	1.10%	0.153%




Sum of corrected areas: 3107517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050325.D
Acq On : 13 Aug 2022 17:53
Operator : SY/MD
Sample : N4065-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

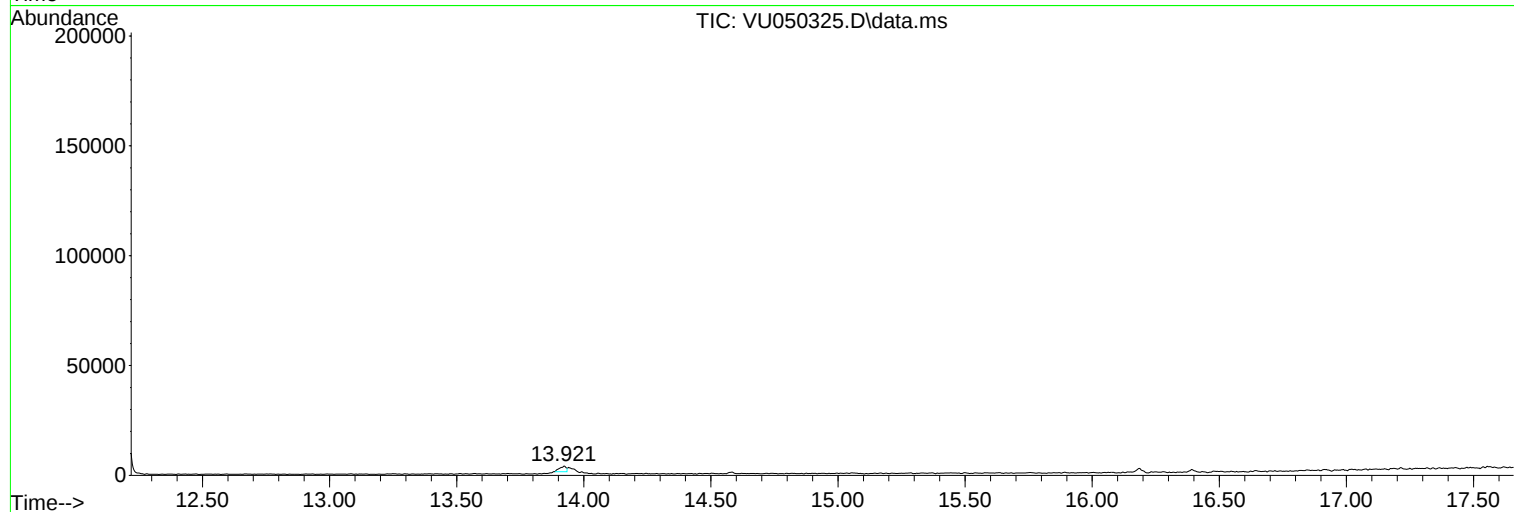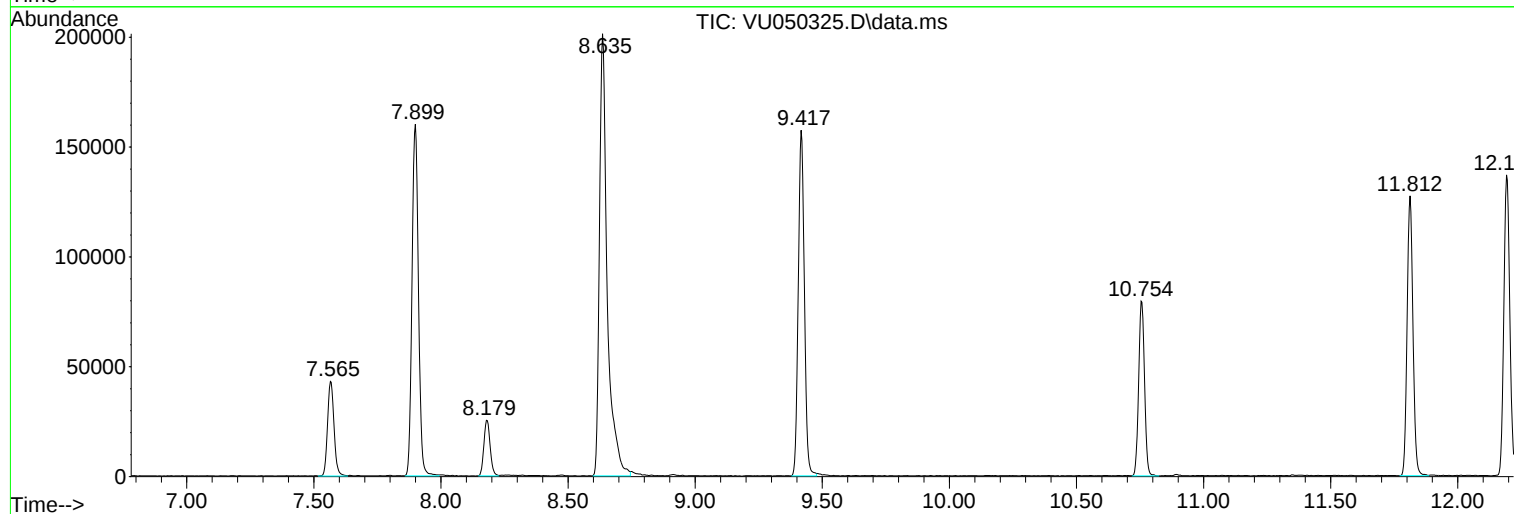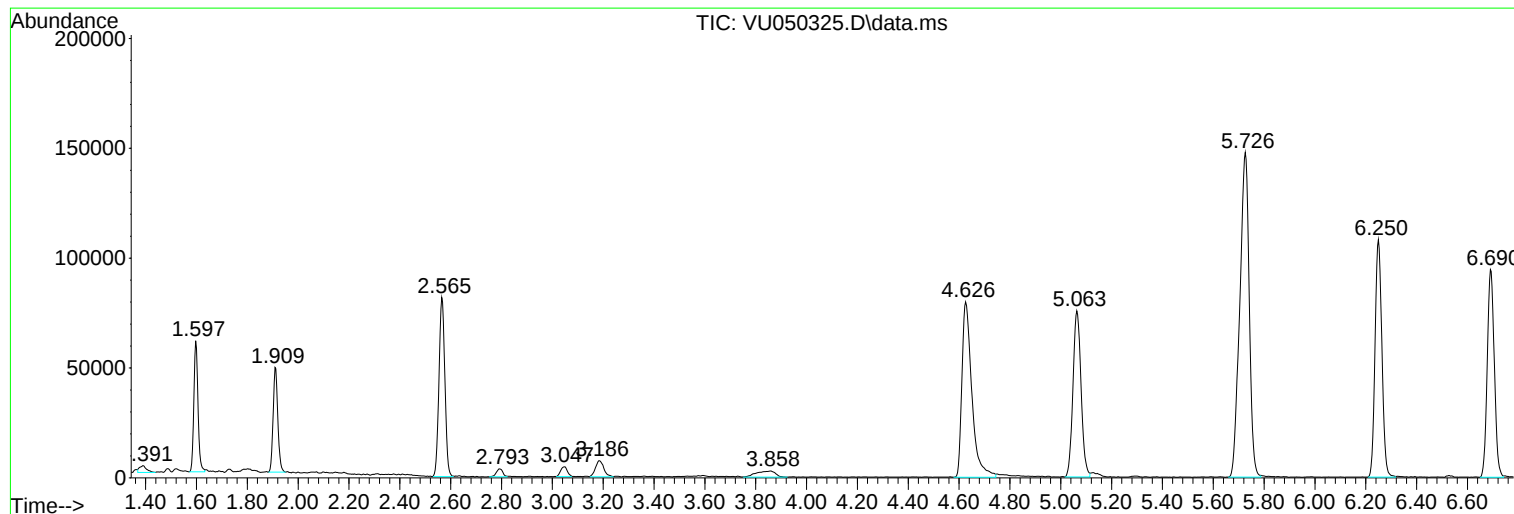

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050325.D
Acq On : 13 Aug 2022 17:53
Operator : SY/MD
Sample : N4065-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
Data File : VU050325.D
Acq On : 13 Aug 2022 17:53
Operator : SY/MD
Sample : N4065-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
