


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081322\
 Data File : VU050310.D
 Acq On : 13 Aug 2022 09:14
 Operator : SY/MD
 Sample : BFB104
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB104

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sun Aug 14 01:24:58 2022

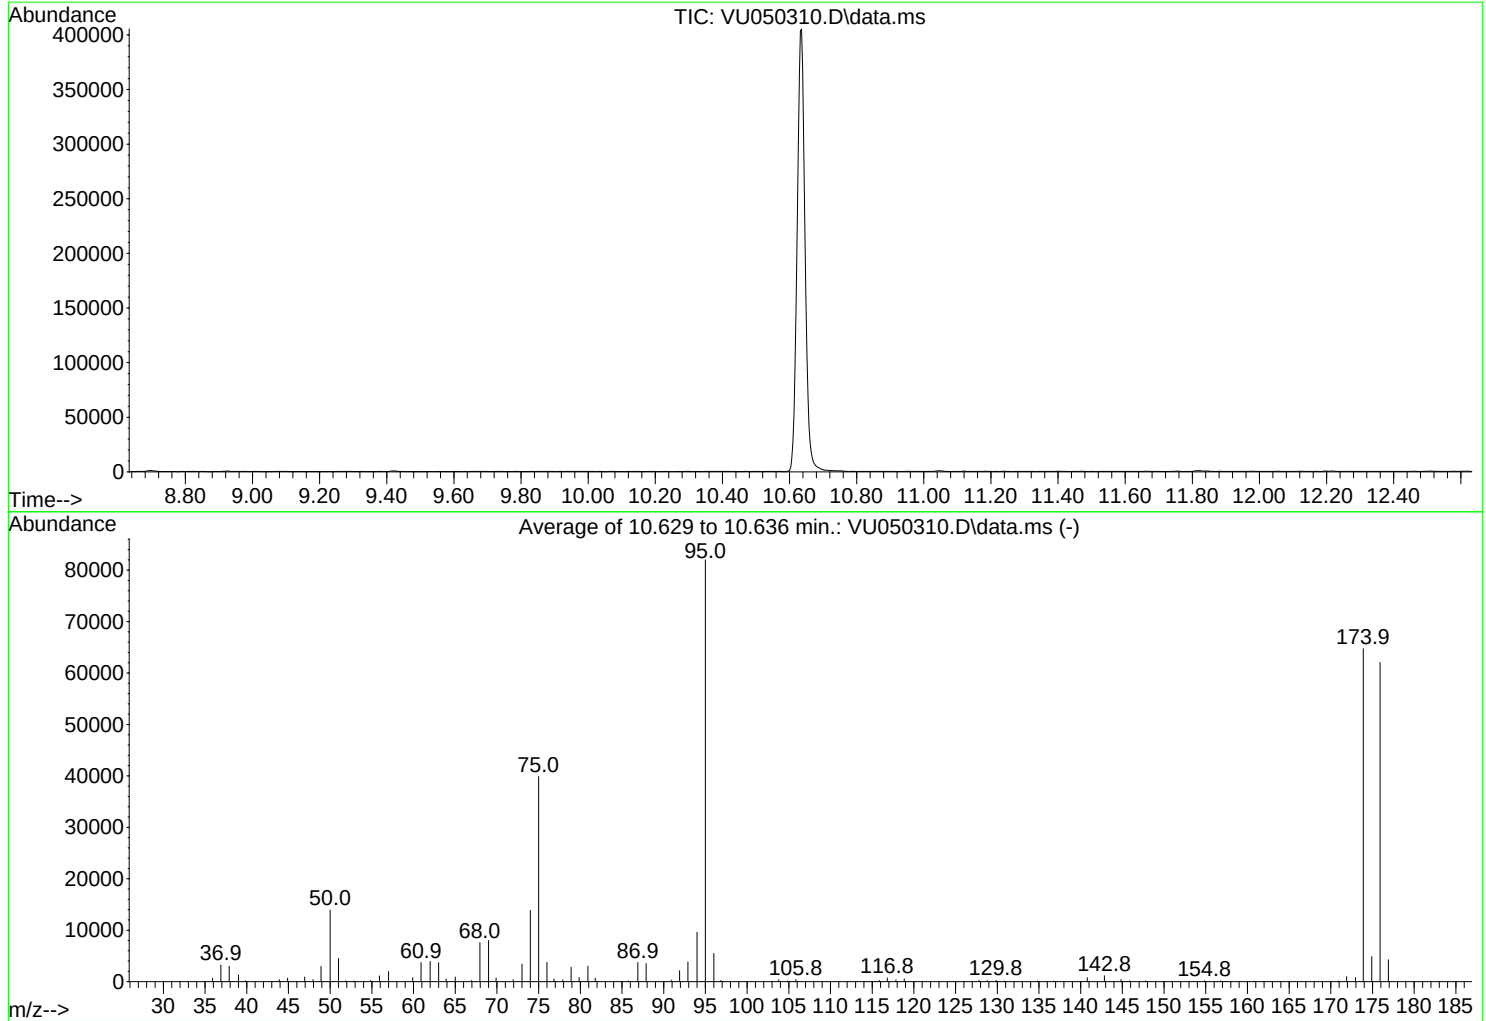

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	13909	PASS
75	95	30	80	48.6	39872	PASS
95	95	100	100	100.0	82005	PASS
96	95	5	9	6.7	5484	PASS
173	174	0.00	2	1.2	766	PASS
174	95	50	120	78.9	64739	PASS
175	174	5	9	7.5	4843	PASS
176	174	95	101	95.9	62069	PASS
177	176	5	9	6.9	4258	PASS

m/z	Abundance
43.90	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	615.0
36.90	2958.0
37.90	2843.0
39.00	1255.0
39.90	157.0
43.90	556.0
44.90	609.0
46.90	896.0
48.00	367.0
48.90	2735.0
50.00	13151.0
51.00	4361.0
51.90	224.0
52.90	109.0
54.80	172.0
55.90	1186.0
57.00	1851.0
59.90	689.0
60.90	3434.0
62.00	3758.0
63.00	3423.0
63.90	502.0
65.00	876.0
67.00	227.0
68.00	7207.0
69.00	7594.0
69.90	693.0
72.00	368.0
73.00	3311.0
74.00	13365.0
75.00	37440.0
76.00	3388.0
76.80	568.0
77.90	321.0
78.90	2618.0
79.80	789.0
80.90	2906.0
81.80	655.0
85.70	113.0
86.90	3456.0
87.90	3140.0
90.90	261.0
91.90	2025.0
92.90	3381.0
94.00	8811.0
95.00	77008.0
96.00	5182.0
96.90	228.0
103.80	351.0
104.90	133.0
105.90	339.0
115.80	240.0
116.80	660.0
117.80	348.0
118.80	464.0
127.80	202.0
128.80	240.0
129.80	258.0
130.90	130.0
134.90	124.0
136.80	125.0
140.80	702.0
142.80	1126.0
144.90	424.0
145.90	139.0
147.80	131.0
154.90	171.0
156.80	146.0
160.80	135.0
170.90	136.0
171.90	932.0
173.00	804.0
173.90	59312.0
174.90	4441.0
175.90	56736.0
176.90	3943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	656.0
36.90	3391.0
37.90	3111.0
39.00	1360.0
39.90	173.0
43.90	597.0
44.90	728.0
46.00	105.0
47.00	933.0
48.00	407.0
48.90	3085.0
50.00	14309.0
51.00	4695.0
51.90	195.0
52.80	128.0
54.80	207.0
55.90	1159.0
57.00	2043.0
59.90	803.0
60.90	3802.0
62.00	4062.0
63.00	3833.0
63.90	567.0
65.00	934.0
66.90	234.0
68.00	7788.0
69.00	8230.0
69.90	763.0
71.90	409.0
73.00	3518.0
74.00	14262.0
75.00	41064.0
76.00	3863.0
76.90	540.0
77.90	372.0
78.90	2893.0
79.80	815.0
80.90	3098.0
81.80	691.0
85.70	174.0
86.90	3864.0
87.90	3609.0
90.90	290.0
91.90	2141.0
92.90	3987.0
94.00	9910.0
95.00	84600.0
96.00	5705.0
96.90	206.0
103.80	386.0
104.90	156.0
105.80	419.0
115.80	257.0
116.80	735.0
117.80	348.0
118.80	567.0
127.80	256.0
128.80	227.0
129.90	281.0
130.90	118.0
134.80	150.0
136.80	134.0
140.80	820.0
142.80	1184.0
144.80	419.0
145.90	191.0
147.80	156.0
154.80	188.0
156.80	181.0
160.80	124.0
170.90	137.0
171.90	997.0
173.00	765.0
173.90	66784.0
174.90	5011.0
175.90	63856.0
176.90	4380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	624.0
36.90	3360.0
37.90	3038.0
39.00	1317.0
39.80	197.0
43.90	658.0
44.90	719.0
46.90	902.0
47.90	420.0
48.90	3061.0
50.00	14268.0
51.00	4445.0
51.90	173.0
52.80	125.0
54.90	244.0
55.90	1045.0
57.00	2002.0
59.90	837.0
60.90	3908.0
62.00	3976.0
63.00	3742.0
63.90	563.0
65.00	869.0
67.00	203.0
67.90	7789.0
69.00	8142.0
69.90	702.0
72.00	389.0
73.00	3454.0
74.00	13876.0
75.00	41112.0
76.00	3952.0
76.90	502.0
77.90	381.0
78.90	2926.0
79.90	785.0
80.90	2925.0
81.80	682.0
85.80	204.0
86.90	3782.0
87.90	3844.0
90.90	318.0
91.90	2154.0
92.90	4108.0
94.00	10021.0
95.00	84408.0
96.00	5564.0
96.80	190.0
103.80	399.0
104.80	145.0
105.80	458.0
115.90	261.0
116.80	727.0
117.90	336.0
118.90	597.0
127.80	307.0
128.80	191.0
129.90	291.0
130.90	119.0
134.80	171.0
136.80	150.0
140.80	814.0
142.00	107.0
142.90	1142.0
144.80	373.0
145.90	214.0
147.80	173.0
154.80	173.0
156.80	197.0
170.90	150.0
171.90	952.0
172.90	729.0
173.90	68120.0
174.90	5076.0
175.90	65616.0
176.90	4450.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104