

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081324\
 Data File : VU060432.D
 Acq On : 13 Aug 2024 18:08
 Operator : MD/SY
 Sample : P3501-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBX2

Quant Time: Aug 14 01:24:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 14 01:18:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	81897	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	87721	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	38514	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	21083	3.280	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.600%
7) Chloroethane-d5	1.911	69	23348	4.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	2.560	65	9963	3.642	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.800%
20) 2-Butanone-d5	4.631	46	81451	59.702	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.400%
24) Chloroform-d	5.055	84	59493	4.674	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.695	65	31560	5.347	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	5.721	84	106306	4.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%
36) 1,2-Dichloropropane-d6	6.682	67	37700	4.594	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.800%
41) Toluene-d8	7.894	98	86167	3.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	8.177	79	11274	4.250	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.631	63	58981	50.099	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.200%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	32362	4.806	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	36016	5.076	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						
13) Acetone	2.644	43	29641	31.816	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081324\
Data File : VU060432.D
Acq On : 13 Aug 2024 18:08
Operator : MD/SY
Sample : P3501-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BX2

Quant Time: Aug 14 01:24:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 14 01:18:59 2024
Response via : Initial Calibration

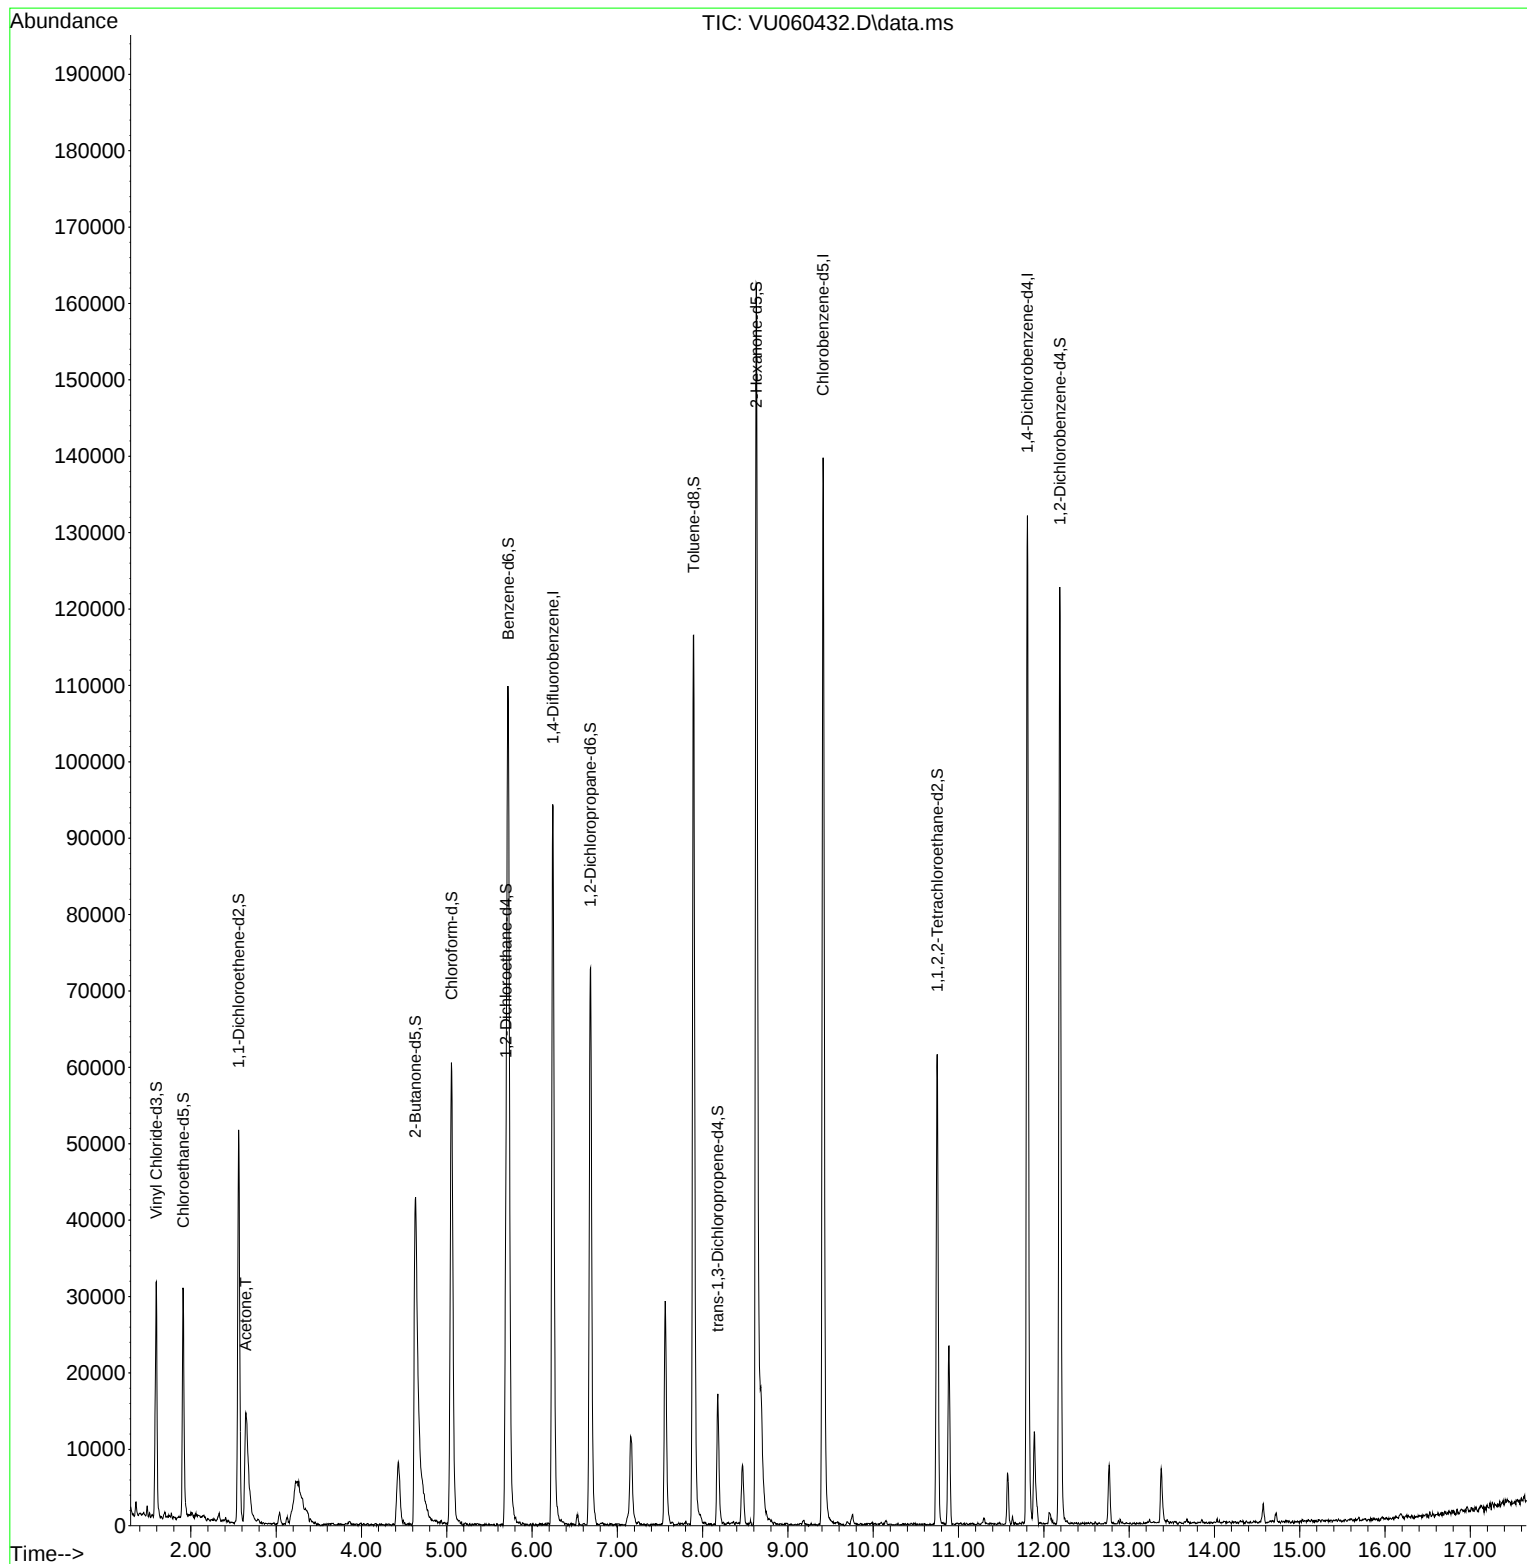

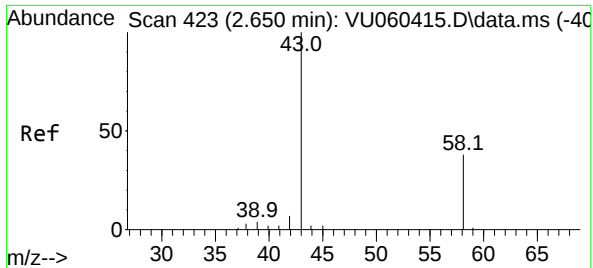

#13
 Acetone
 Concen: 31.816 ug/L
 RT: 2.644 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU060432.D
 Acq: 13 Aug 2024 18:08

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BX2

Tgt Ion: 43 Resp: 29641
 Ion Ratio Lower Upper
 43 100
 58 36.6 0.0 78.8

