


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081324\
Data File : VU060413.D
Acq On : 13 Aug 2024 09:20
Operator : MD/SY
Sample : BFB184
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB184

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Aug 14 01:18:59 2024

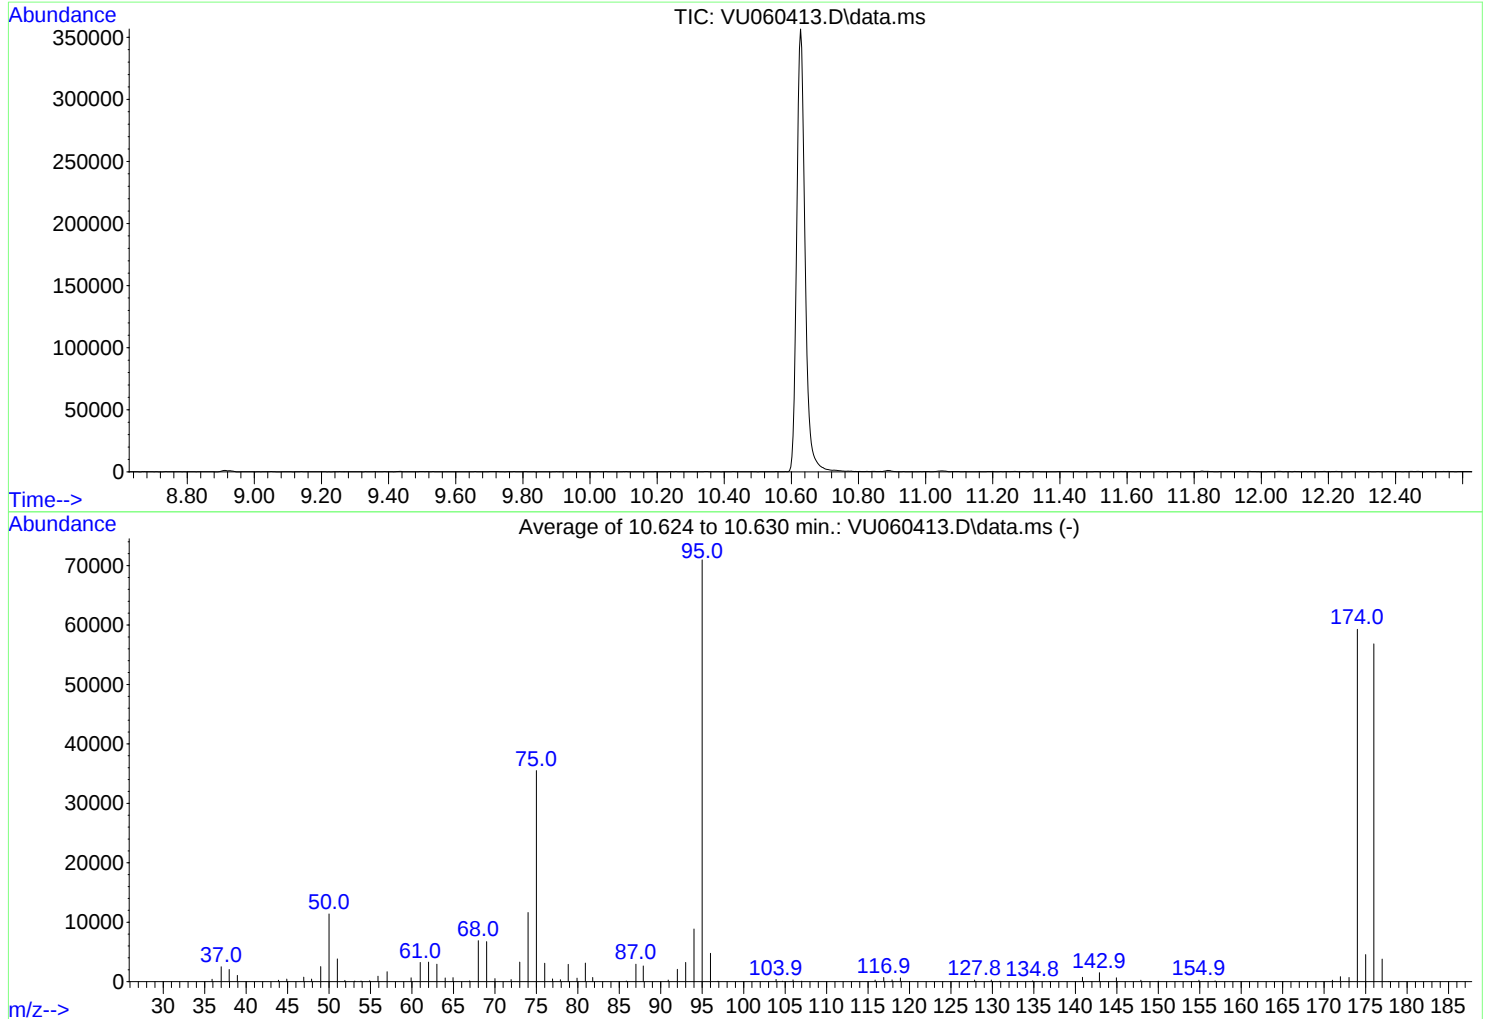

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	11392	PASS
75	95	30	80	50.0	35517	PASS
95	95	100	100	100.0	70968	PASS
96	95	5	9	6.7	4767	PASS
173	174	0.00	2	1.2	715	PASS
174	95	50	120	83.5	59283	PASS
175	174	5	9	7.7	4560	PASS
176	174	95	101	95.9	56840	PASS
177	176	5	9	6.7	3799	PASS

m/z	Abundance
39.90	106.0
43.90	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.90	360.0
37.00	2591.0
38.00	2029.0
39.00	1101.0
44.00	436.0
44.90	432.0
46.90	669.0
47.90	404.0
49.00	2602.0
50.00	11430.0
51.00	3832.0
51.90	253.0
53.10	102.0
53.90	103.0
54.90	219.0
55.90	958.0
57.00	1595.0
59.90	702.0
61.00	3204.0
62.00	3387.0
63.00	2921.0
64.00	680.0
65.00	711.0
67.00	104.0
68.00	6877.0
69.00	6651.0
70.00	551.0
72.00	360.0
73.00	3172.0
74.00	11502.0
75.00	35248.0
76.00	3082.0
77.00	405.0
77.90	288.0
78.80	2871.0
79.90	642.0
80.90	3113.0
81.80	702.0
85.90	170.0
87.00	2922.0
87.90	2546.0
90.90	263.0
92.00	1873.0
93.00	3150.0
94.00	8709.0
95.00	69384.0
96.00	4923.0
103.90	364.0
104.70	118.0
106.00	287.0
115.90	267.0
116.90	723.0
117.90	293.0
118.90	557.0
127.80	281.0
129.90	281.0
130.90	106.0
134.90	114.0
140.90	773.0
142.90	1425.0
144.90	680.0
147.90	260.0
154.90	265.0
156.80	159.0
171.00	235.0
172.00	802.0
173.00	1110.0
174.00	57368.0
175.00	4494.0
176.00	55264.0
177.00	3832.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.90	416.0
37.00	2566.0
37.90	2087.0
38.90	1057.0
43.90	397.0
44.90	454.0
47.00	803.0
47.90	453.0
49.00	2649.0
50.00	11697.0
51.00	3976.0
51.90	227.0
53.10	134.0
53.90	109.0
54.90	174.0
55.90	966.0
57.00	1746.0
59.90	648.0
61.00	3329.0
62.00	3367.0
63.00	2995.0
64.00	655.0
65.00	679.0
66.90	125.0
68.00	7091.0
69.00	6912.0
70.00	494.0
71.90	360.0
73.00	3367.0
74.00	11940.0
75.00	36640.0
76.00	3181.0
77.00	453.0
77.90	357.0
78.90	2983.0
79.90	609.0
80.90	3255.0
81.80	739.0
85.80	122.0
87.00	3055.0
87.90	2716.0
90.90	296.0
92.00	2138.0
93.00	3354.0
94.00	9059.0
95.00	72888.0
96.00	4920.0
96.90	119.0
103.90	392.0
104.70	129.0
106.00	303.0
107.00	108.0
115.90	279.0
116.90	705.0
117.90	322.0
118.90	631.0
127.90	286.0
129.90	265.0
130.90	114.0
134.90	138.0
140.80	749.0
141.90	103.0
142.90	1581.0
145.00	678.0
147.90	270.0
150.00	132.0
154.90	263.0
156.80	146.0
171.00	251.0
171.90	834.0
173.00	1035.0
174.00	60888.0
175.00	4677.0
176.00	58528.0
177.00	3945.0
177.80	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.90	479.0
37.00	2346.0
38.00	2031.0
38.90	970.0
40.00	132.0
43.90	352.0
44.90	436.0
46.90	821.0
47.90	419.0
49.00	2312.0
50.00	11049.0
51.00	3705.0
51.90	172.0
53.10	128.0
53.80	103.0
54.90	122.0
55.90	865.0
57.00	1698.0
59.90	608.0
61.00	3158.0
62.00	3144.0
63.00	2914.0
64.00	571.0
64.90	662.0
66.90	176.0
68.00	6679.0
69.00	6596.0
70.00	485.0
71.90	357.0
73.00	3302.0
74.00	11417.0
75.00	34664.0
76.00	3050.0
76.90	528.0
77.90	350.0
78.90	2843.0
79.90	565.0
80.90	3031.0
81.80	681.0
87.00	2831.0
87.90	2685.0
90.90	280.0
92.00	2194.0
93.00	3202.0
94.00	8810.0
95.00	70632.0
96.00	4459.0
96.90	116.0
103.90	350.0
105.80	280.0
107.00	121.0
115.80	293.0
116.90	661.0
117.90	288.0
118.90	649.0
127.90	281.0
129.80	251.0
134.80	152.0
136.90	123.0
140.80	674.0
142.90	1538.0
145.00	595.0
147.90	218.0
150.00	144.0
154.90	209.0
156.90	110.0
171.00	272.0
171.90	841.0
174.00	59592.0
175.00	4510.0
176.00	56728.0
177.00	3621.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184