




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081325\
Data File : VU063555.D
Acq On : 13 Aug 2025 10:05
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Quant Time: Aug 13 22:39:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 13 22:38:52 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/18/2025
Supervised By :Semsettin Yesilyurt 08/18/2025

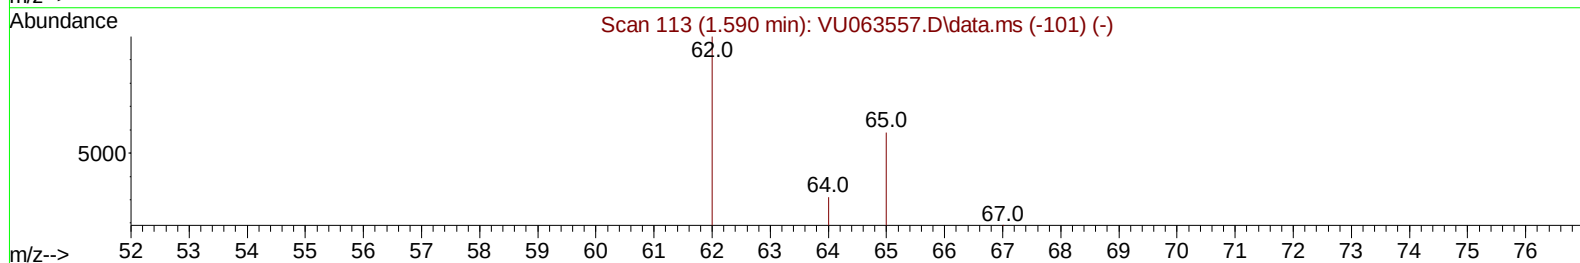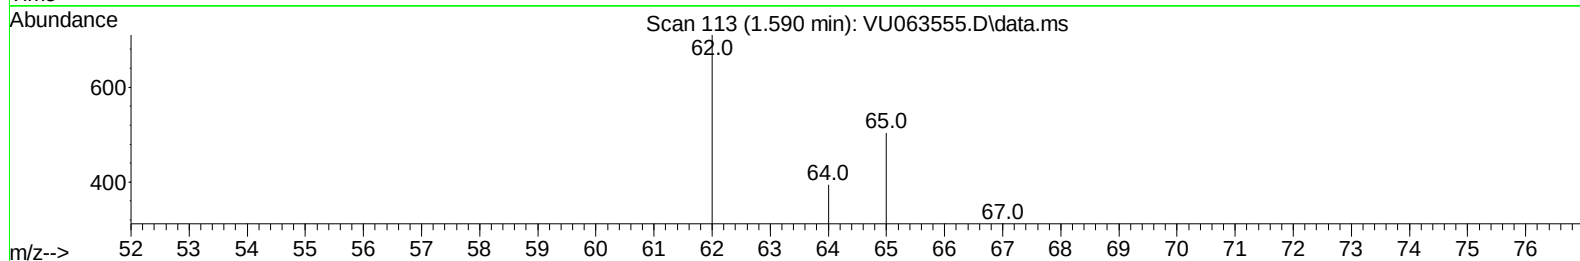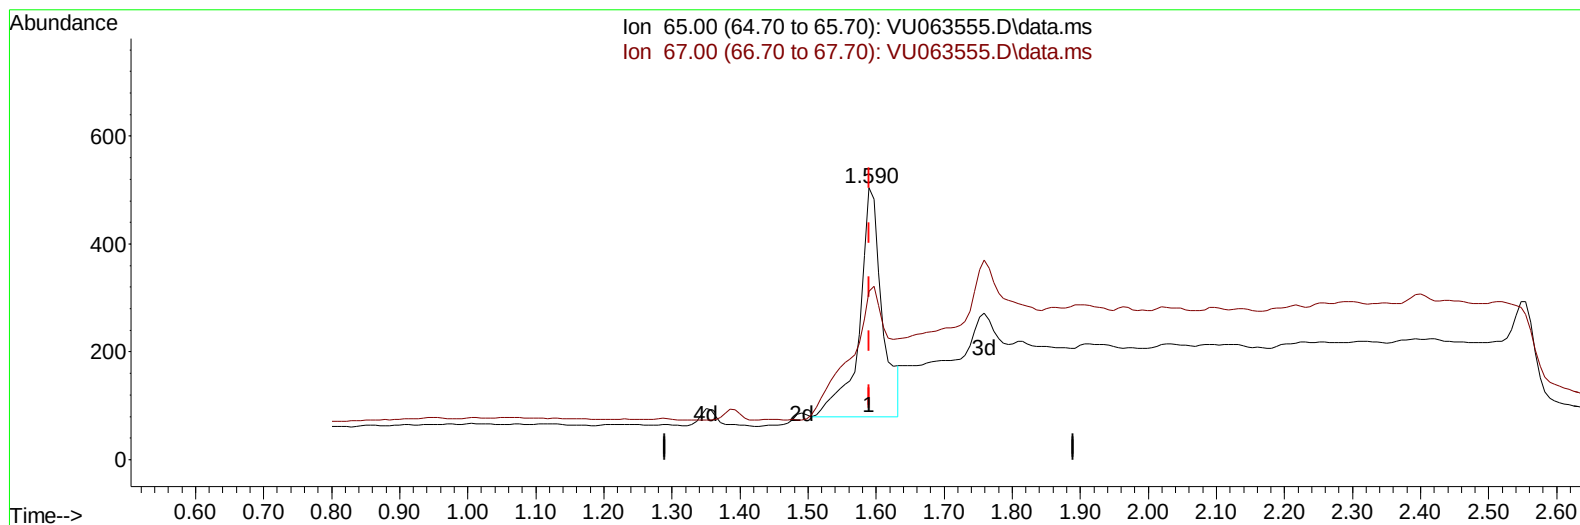

TIC: VU063555.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.590min (-0.000) 0.08 ug/L

response 1006

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	39.70	93.34#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081325\
Data File : VU063555.D
Acq On : 13 Aug 2025 10:05
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Quant Time: Aug 13 22:39:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 13 22:38:52 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/18/2025
Supervised By :Semsettin Yesilyurt 08/18/2025

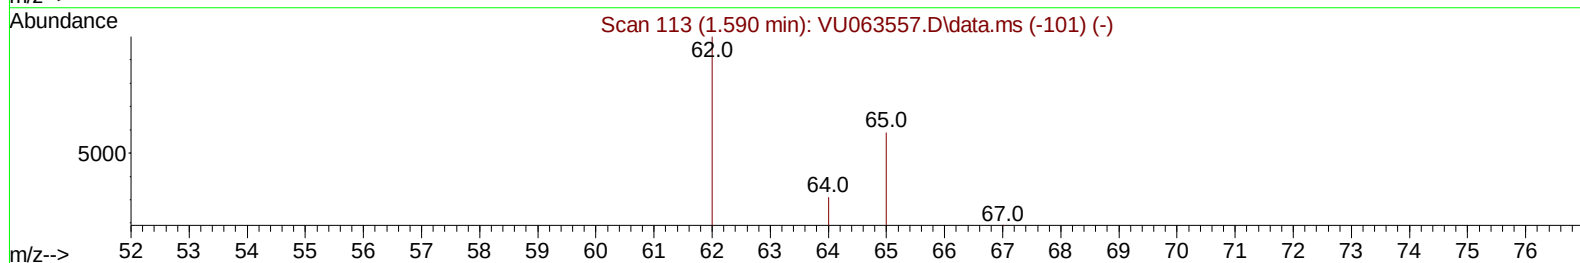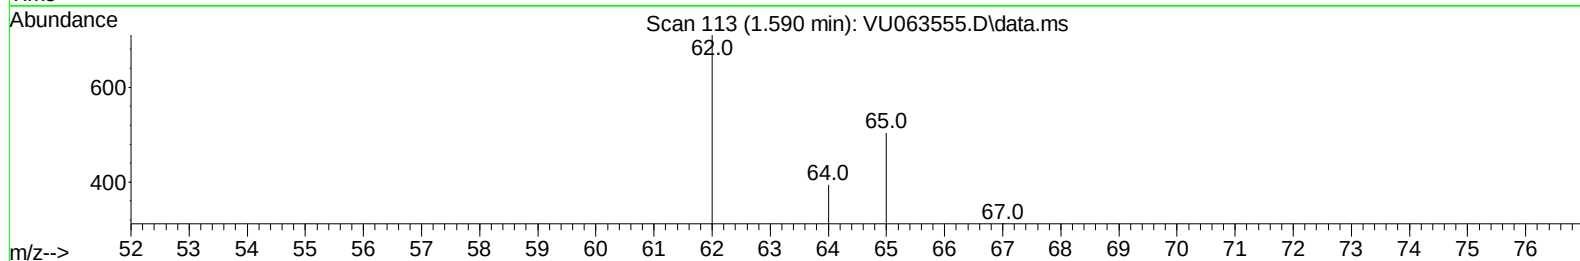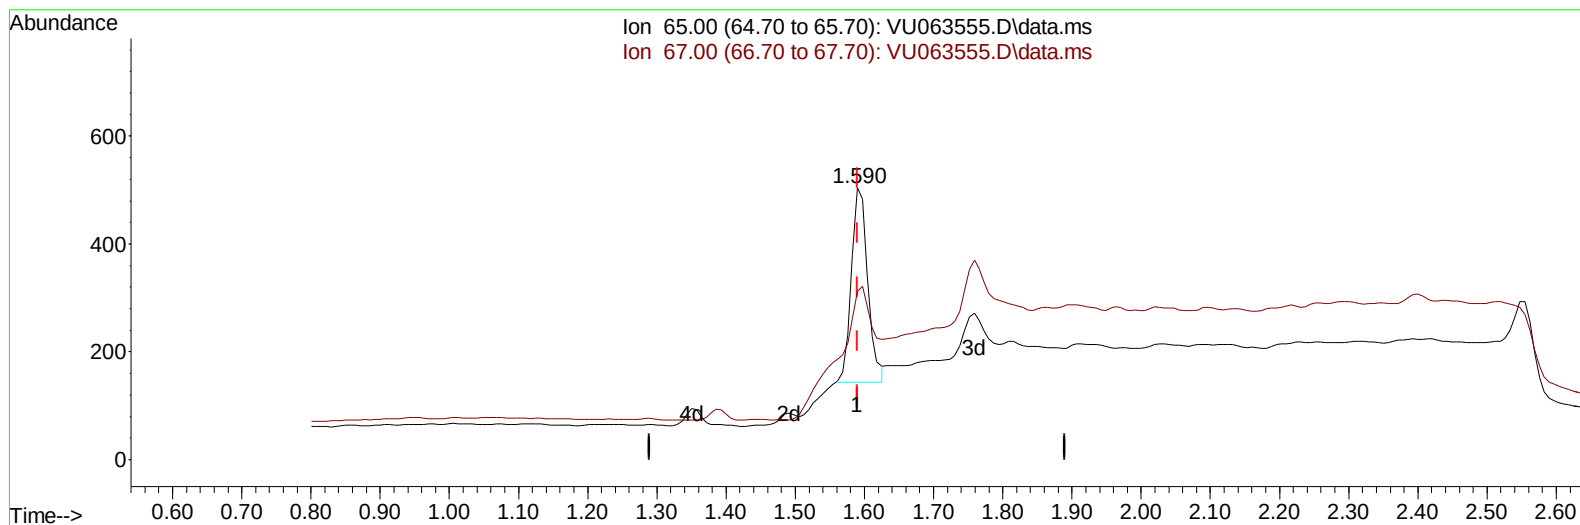

TIC: VU063555.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.590min (-0.000) 0.04 ug/L m

response 594

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	39.70	158.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081325\
 Data File : VU063555.D
 Acq On : 13 Aug 2025 10:05
 Operator : MD/SY
 Sample : VSTD0.0562
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.05062

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/18/2025
 Supervised By :Semsettin Yesilyurt 08/18/2025

Quant Time: Aug 13 22:39:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081325.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 13 22:38:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	19299	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	25016	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152	8629	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	594m	0.044	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.709	65	455	0.062	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.687	67	292	0.045	ug/L	0.00
8) Toluene-d8	7.903	98	1133	0.052	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.745	84	239	0.048	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.597	62	1318	0.062	ug/L #	64
6) Trichloroethene	6.544	95	969	0.064	ug/L	94
9) 1,2-Dibromoethane	8.924	107	428	0.051	ug/L #	94
12) 1,2,3-Trichloropropane	10.814	75	406	0.054	ug/L #	73
13) 1,2-Dibromo-3-chloropr...	13.007	75	83	0.063	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081325\
Data File : VU063555.D
Acq On : 13 Aug 2025 10:05
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Quant Time: Aug 13 22:39:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 13 22:38:52 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/18/2025
Supervised By :Semsettin Yesilyurt 08/18/2025

