


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081325\
Data File : VU063554.D
Acq On : 13 Aug 2025 08:37
Operator : MD/SY
Sample : BFB026
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB026

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM081325.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 13 22:46:04 2025

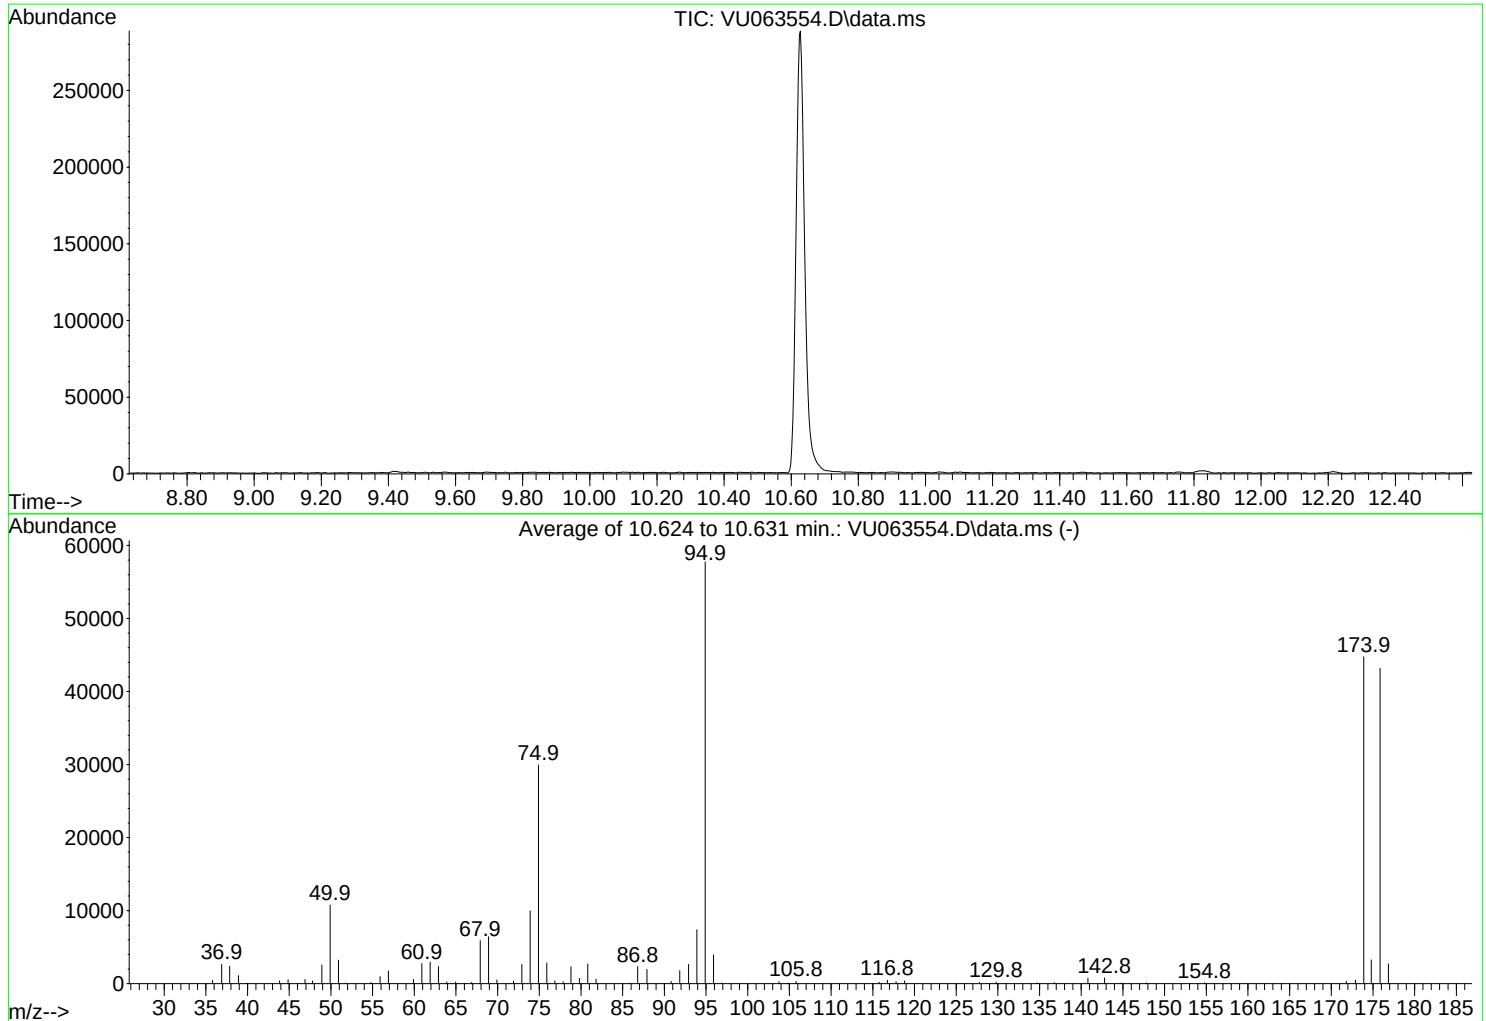

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	10758	PASS
75	95	30	80	51.8	29925	PASS
95	95	100	100	100.0	57757	PASS
96	95	5	9	6.8	3934	PASS
173	174	0.00	2	1.1	478	PASS
174	95	50	120	77.5	44755	PASS
175	174	5	9	7.3	3248	PASS
176	174	95	101	96.5	43179	PASS
177	176	5	9	6.3	2718	PASS

m/z	Abundance
35.80	388.0
37.80	115.0
40.00	115.0
43.80	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	839.0
36.90	2731.0
37.90	2521.0
38.90	1171.0
39.80	118.0
43.90	611.0
44.90	500.0
46.90	597.0
47.80	388.0
48.90	2681.0
49.90	11229.0
50.90	3287.0
51.70	153.0
54.80	185.0
55.90	949.0
56.90	1835.0
59.90	631.0
60.90	2713.0
61.90	3073.0
62.90	2396.0
63.90	279.0
64.90	197.0
66.90	144.0
67.90	6032.0
68.90	6541.0
69.90	484.0
71.90	329.0
72.90	2727.0
73.90	10191.0
74.90	31064.0
75.90	2776.0
76.80	385.0
77.80	257.0
78.80	2472.0
79.80	738.0
80.80	2689.0
81.80	614.0
85.80	106.0
86.80	2334.0
87.90	2065.0
90.80	299.0
91.80	1779.0
92.90	2711.0
93.90	7453.0
94.90	59024.0
95.90	3951.0
96.80	154.0
103.70	266.0
104.80	105.0
105.80	325.0
115.80	201.0
116.80	441.0
117.80	259.0
118.80	390.0
127.80	171.0
129.80	211.0
134.70	101.0
136.80	135.0
140.80	710.0
142.80	820.0
145.70	100.0
147.80	115.0
154.80	133.0
171.80	361.0
172.90	496.0
173.90	44872.0
174.80	3343.0
175.80	43464.0
176.80	2807.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	841.0
36.90	2713.0
37.90	2526.0
38.90	1160.0
39.80	119.0
43.90	617.0
44.80	549.0
46.90	615.0
47.80	379.0
48.90	2681.0
49.90	11074.0
50.90	3296.0
51.80	105.0
54.80	164.0
55.90	993.0
56.90	1778.0
59.90	600.0
60.90	2834.0
61.90	3040.0
62.90	2413.0
63.90	265.0
65.00	227.0
66.80	158.0
67.90	6073.0
68.90	6653.0
69.90	494.0
71.90	360.0
72.90	2691.0
73.90	10132.0
74.90	30656.0
75.90	2918.0
76.80	392.0
77.90	274.0
78.80	2382.0
79.80	753.0
80.80	2800.0
81.80	625.0
85.80	111.0
86.80	2403.0
87.90	1980.0
90.80	305.0
91.80	1838.0
92.90	2723.0
93.90	7654.0
94.90	59232.0
95.90	4040.0
96.90	125.0
103.80	279.0
104.80	104.0
105.80	344.0
115.70	187.0
116.70	467.0
117.80	279.0
118.80	396.0
127.80	166.0
129.80	217.0
134.70	124.0
136.70	127.0
140.80	776.0
142.80	827.0
144.80	137.0
147.80	116.0
154.80	145.0
171.80	340.0
172.90	497.0
173.90	46032.0
174.80	3327.0
175.80	44240.0
176.80	2790.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.80	825.0
36.90	2507.0
37.90	2392.0
38.90	963.0
39.80	114.0
43.90	584.0
44.80	521.0
46.90	516.0
47.80	371.0
48.90	2362.0
49.90	9972.0
50.90	3097.0
54.80	137.0
55.90	969.0
56.90	1588.0
59.90	526.0
60.90	2719.0
61.90	2720.0
62.90	2229.0
63.90	207.0
65.00	254.0
66.80	160.0
67.90	5575.0
68.90	6085.0
69.90	517.0
71.90	341.0
72.90	2485.0
73.90	9572.0
74.90	28056.0
75.90	2771.0
76.90	344.0
77.90	271.0
78.80	2134.0
79.80	695.0
80.80	2577.0
81.80	583.0
86.80	2273.0
87.90	1809.0
90.80	289.0
91.90	1696.0
92.90	2487.0
93.90	7055.0
94.90	55016.0
95.90	3811.0
103.80	290.0
105.80	319.0
115.70	188.0
116.70	455.0
117.80	290.0
118.80	338.0
127.80	194.0
128.70	110.0
129.80	213.0
134.70	135.0
136.80	110.0
140.80	764.0
142.80	715.0
144.80	136.0
147.80	103.0
154.80	146.0
171.80	293.0
172.90	441.0
173.90	43360.0
174.80	3075.0
175.90	41832.0
176.90	2557.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026