

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
 Data File : VU026100.D
 Acq On : 14 Aug 2018 14:41
 Operator : MD/SY
 Sample : J4451-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZJ9

Quant Time: Aug 14 14:59:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 11 00:58:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	257231	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	239132	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	103344	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	77349	41.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.28%
7) Chloroethane-d5	1.68	69	69299	46.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.98%
11) 1,1-Dichloroethene-d2	2.27	63	119720	33.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.02%
21) 2-Butanone-d5	4.18	46	146065	93.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.21%
24) Chloroform-d	4.65	84	189395	47.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.31	65	130268	48.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.74%
32) Benzene-d6	5.35	84	361346	48.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.32%
36) 1,2-Dichloropropane-d6	6.33	67	119215	49.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.24%
41) Toluene-d8	7.57	98	322389	45.38	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.76%
43) trans-1,3-Dichloropropene-	7.85	79	57895	47.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.64%
47) 2-Hexanone-d5	8.31	63	101706	93.20	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.20%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	169835	48.34	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.68%
64) 1,2-Dichlorobenzene-d4	11.86	152	129091	50.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.34%


Target Compounds					Qvalue
13) Acetone	2.32	43	2198	2.258 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
Data File : VU026100.D
Acq On : 14 Aug 2018 14:41
Operator : MD/SY
Sample : J4451-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZJ9

Quant Time: Aug 14 14:59:22 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 11 00:58:27 2018
Response via : Initial Calibration

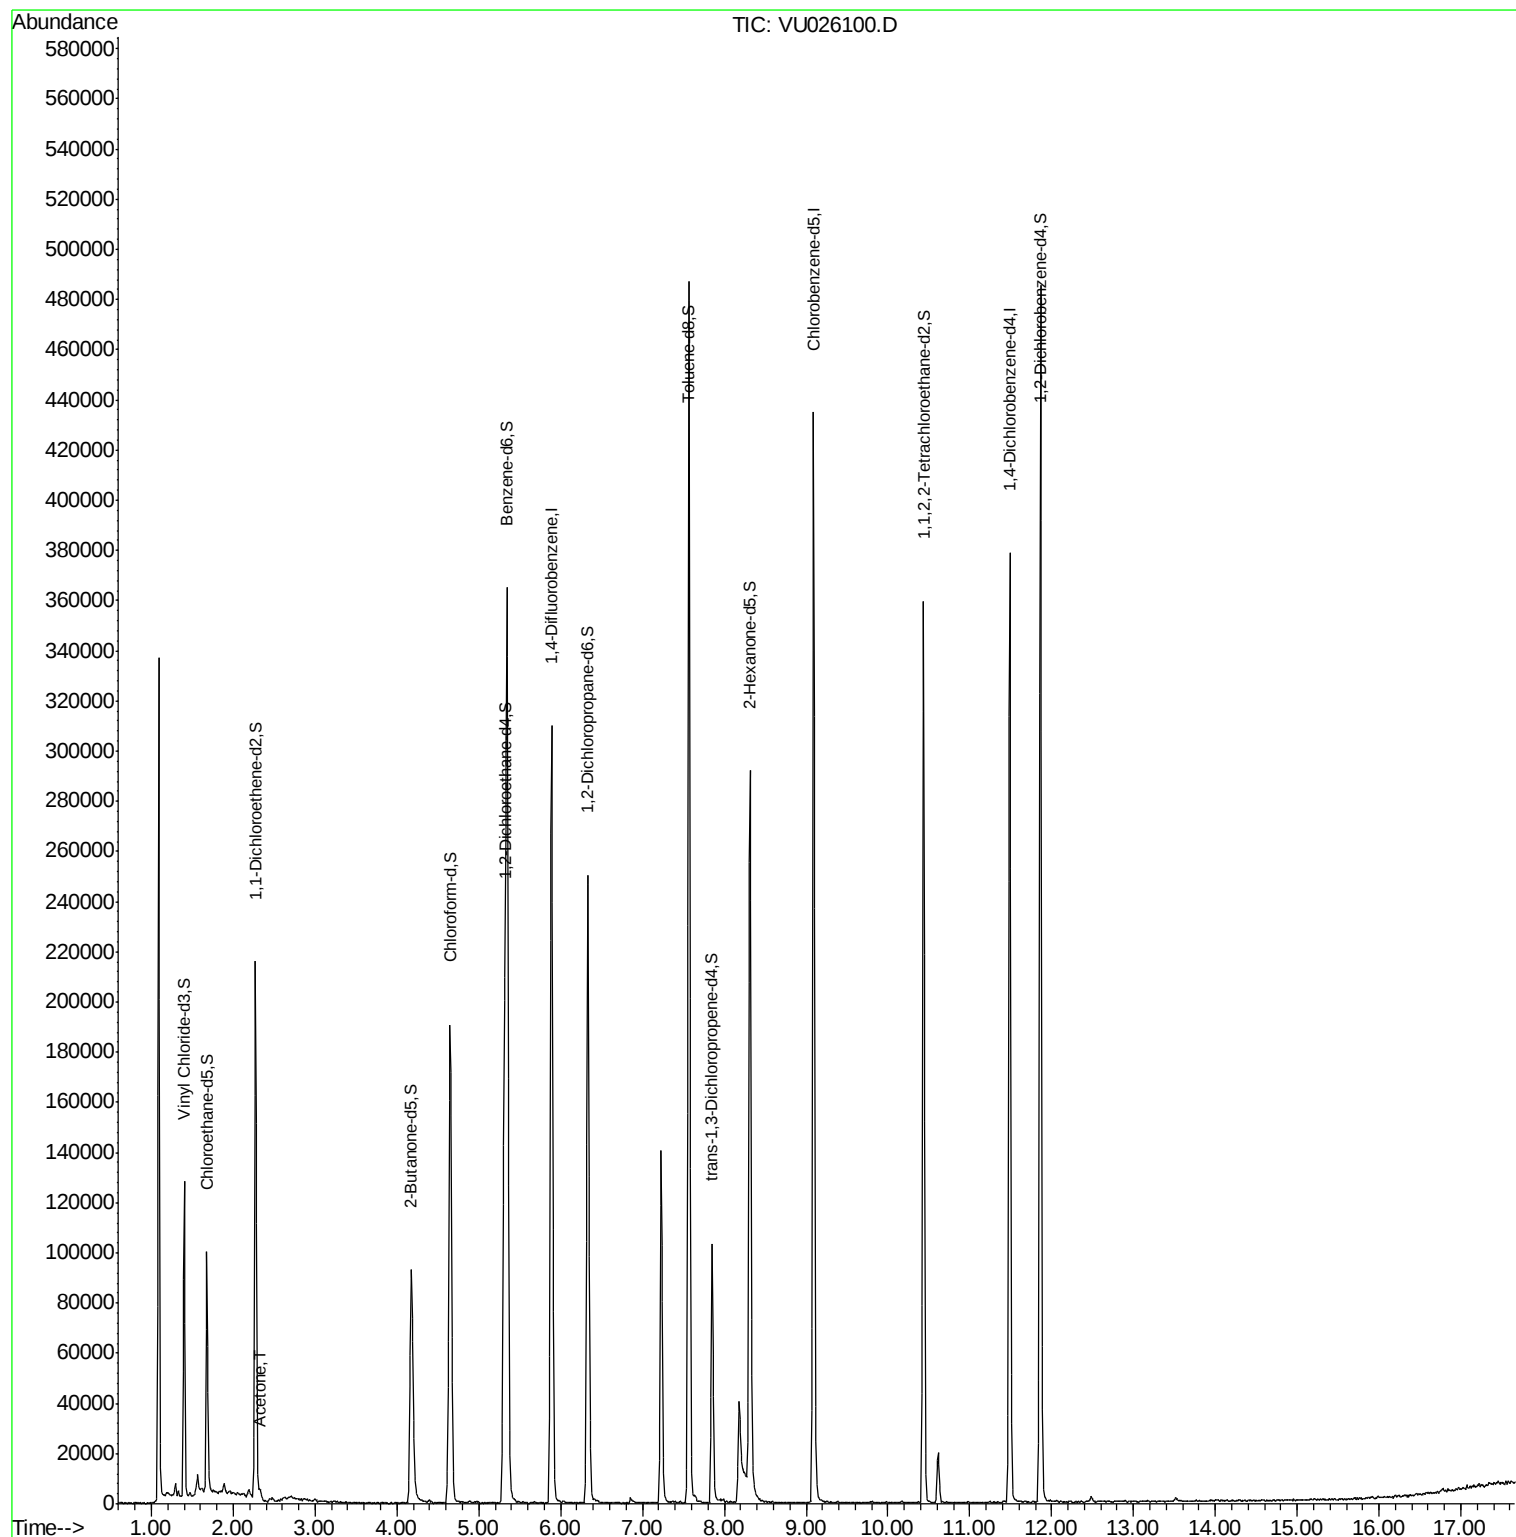

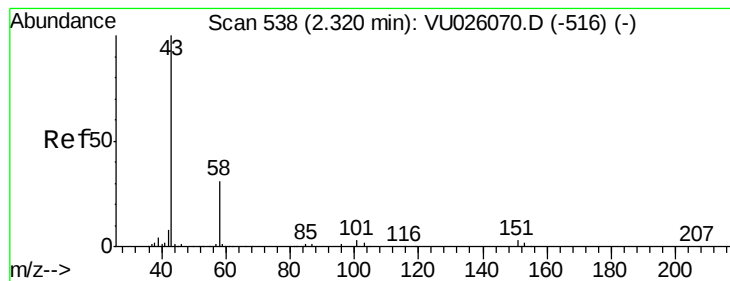

#13

Acetone

Concen: 2.258 ug/L

RT: 2.32 min Scan# 538

Delta R.T. 0.00 min

Lab File: VU026100.D

Acq: 14 Aug 2018 14:41

Instrument :

MSVOA_U

ClientSampleId :


A4ZJ9

Tgt Ion: 43 Resp: 2198

Ion Ratio Lower Upper

43 100

58 19.7 0.0 61.8

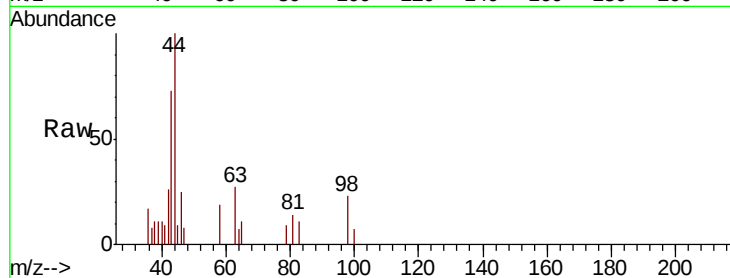

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

