

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
 Data File : VU026101.D
 Acq On : 14 Aug 2018 15:05
 Operator : MD/SY
 Sample : J4451-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4ZK2

Quant Time: Aug 14 15:47:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 11 00:58:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	259173	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	244739	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	103695	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	77716	41.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.04%
7) Chloroethane-d5	1.68	69	68915	45.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.76%
11) 1,1-Dichloroethene-d2	2.27	63	119401	33.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.34%
21) 2-Butanone-d5	4.18	46	147800	93.61	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.61%
24) Chloroform-d	4.65	84	191780	47.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.48%
26) 1,2-Dichloroethane-d4	5.31	65	131201	48.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.70%
32) Benzene-d6	5.35	84	365391	48.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.16%
36) 1,2-Dichloropropane-d6	6.33	67	122513	49.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.64%
41) Toluene-d8	7.57	98	328331	45.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.32%
43) trans-1,3-Dichloropropene-	7.85	79	57000	46.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.02%
47) 2-Hexanone-d5	8.31	63	104198	93.29	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.29%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	169887	47.24	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.48%
64) 1,2-Dichlorobenzene-d4	11.86	152	130596	51.09	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.18%


Target Compounds					Qvalue
13) Acetone	2.32	43	4063	4.142 ug/L	99
48) 2-Hexanone	8.31	43	12723	6.232 ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU081418\
Data File : VU026101.D
Acq On : 14 Aug 2018 15:05
Operator : MD/SY
Sample : J4451-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4ZK2

Quant Time: Aug 14 15:47:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080918WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 11 00:58:27 2018
Response via : Initial Calibration

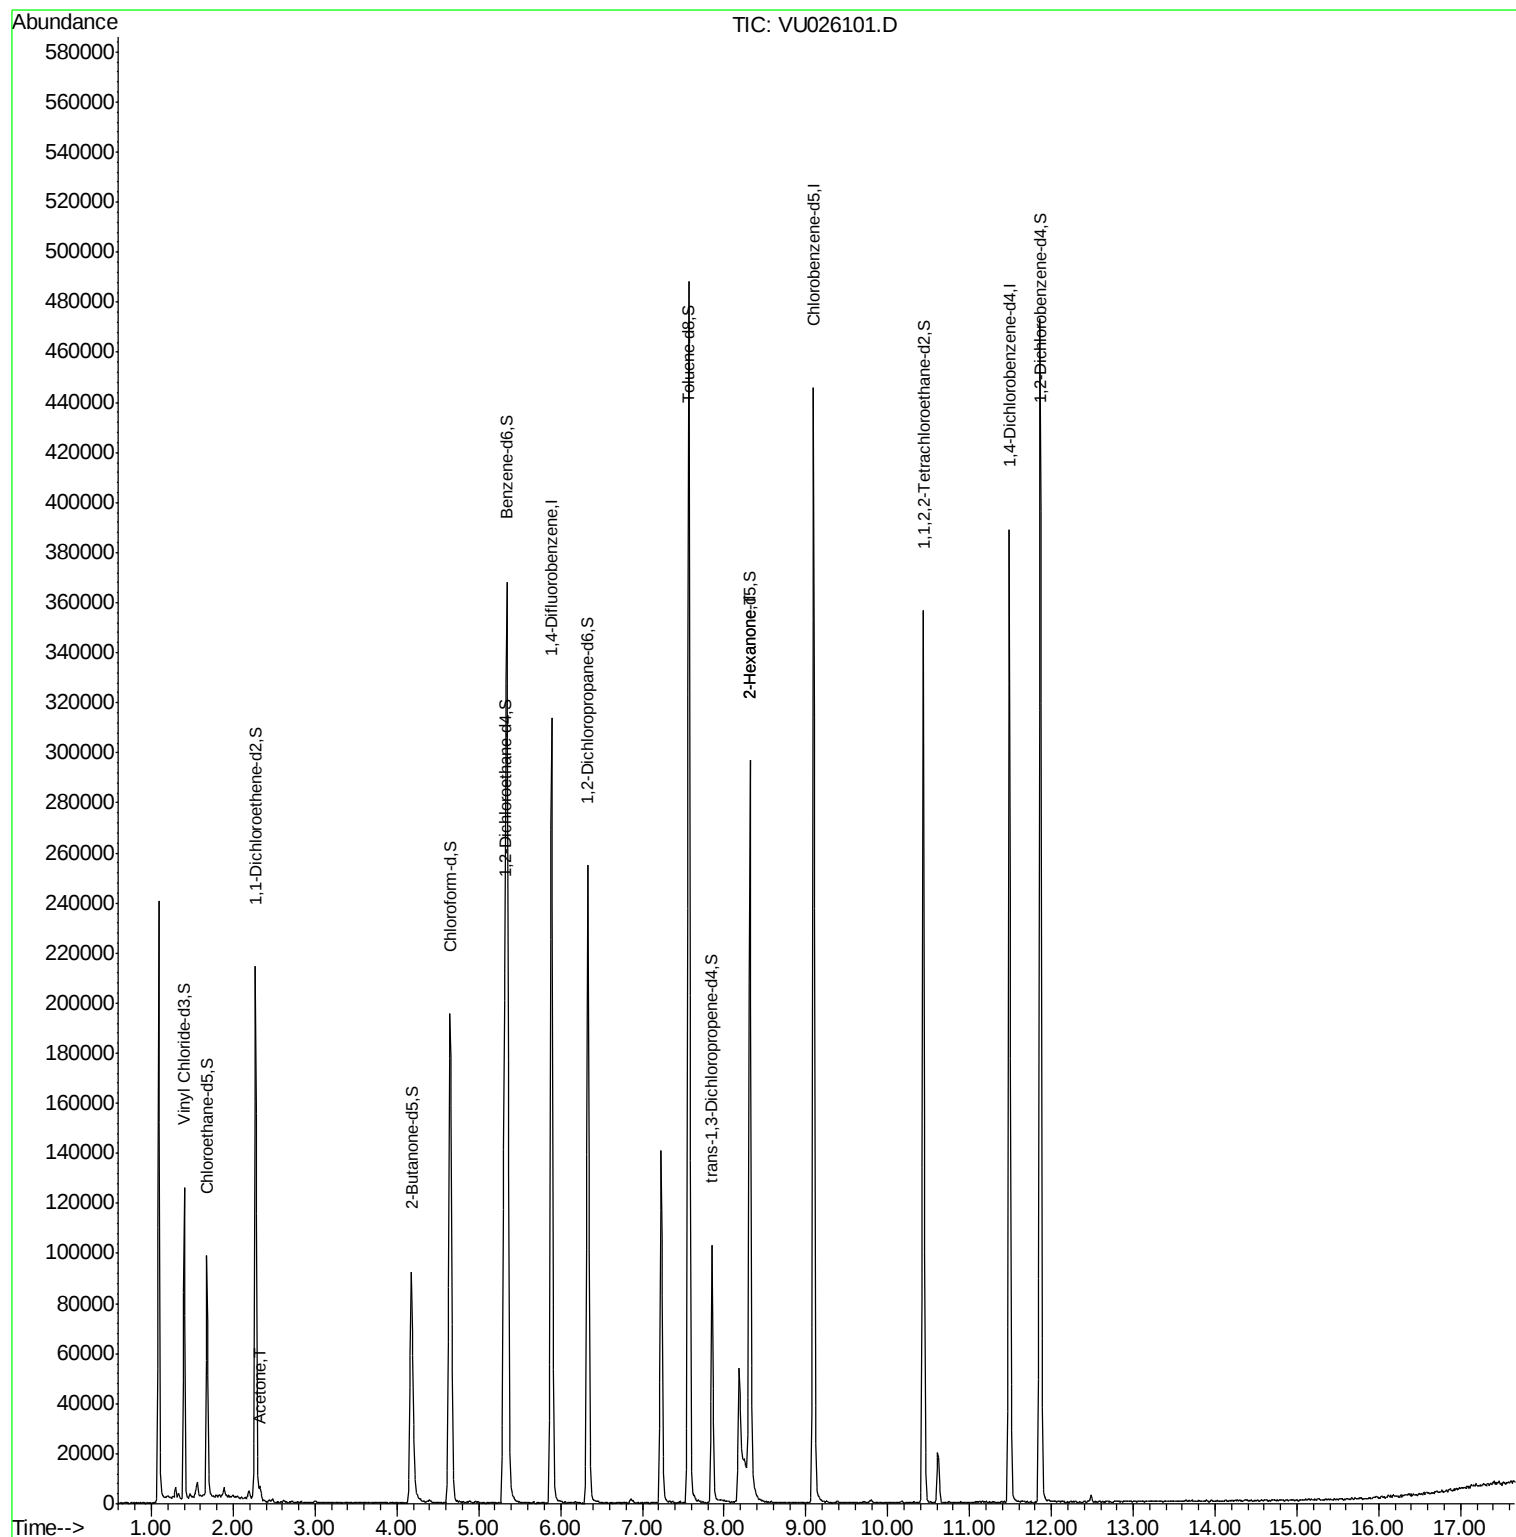

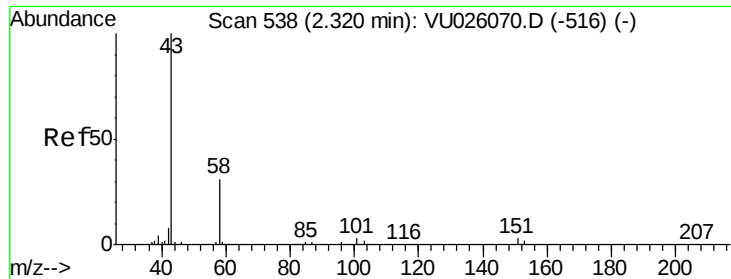

#13

Acetone

Concen: 4.142 ug/L

RT: 2.32 min Scan# 538

Delta R.T. 0.00 min

Lab File: VU026101.D

Acq: 14 Aug 2018 15:05

Instrument :

MSVOA_U

ClientSampleId :


A4ZK2

Tgt Ion: 43 Resp: 4063

Ion Ratio Lower Upper




43 100

58 30.3 0.0 61.8

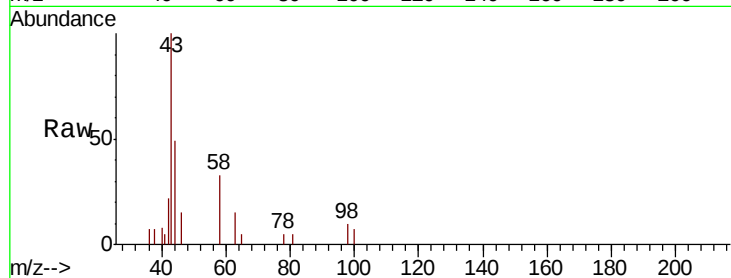

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

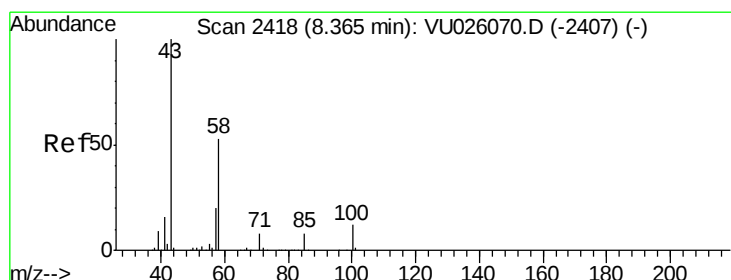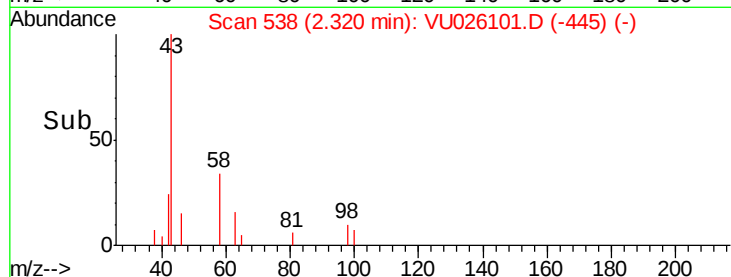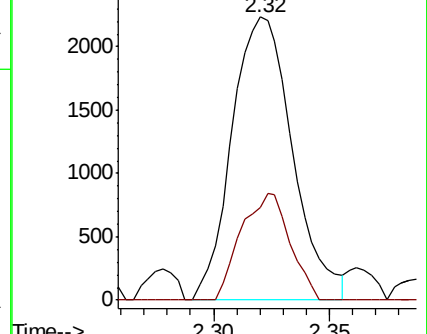

#48

2-Hexanone

Concen: 6.232 ug/L

RT: 8.31 min Scan# 2402

Delta R.T. -0.05 min

Lab File: VU026101.D

Acq: 14 Aug 2018 15:05

Tgt Ion: 43 Resp: 12723


Ion Ratio Lower Upper

43 100

58 24.3 43.6 65.4#

57 28.4 15.1 22.7#

100 0.0 9.3 13.9#

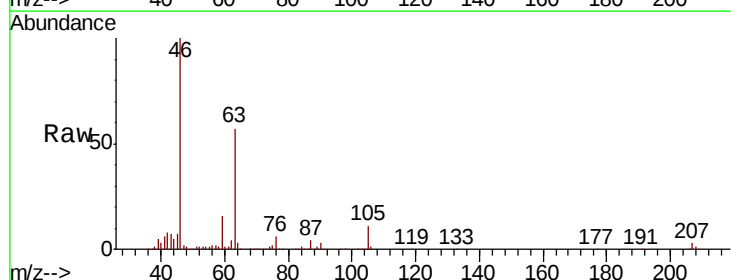

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

Ion 100.00 (99.70 to 100.70): VU0

